


Operating Instructions

Mycom S CLM153

Transmitter for conductivity measurement

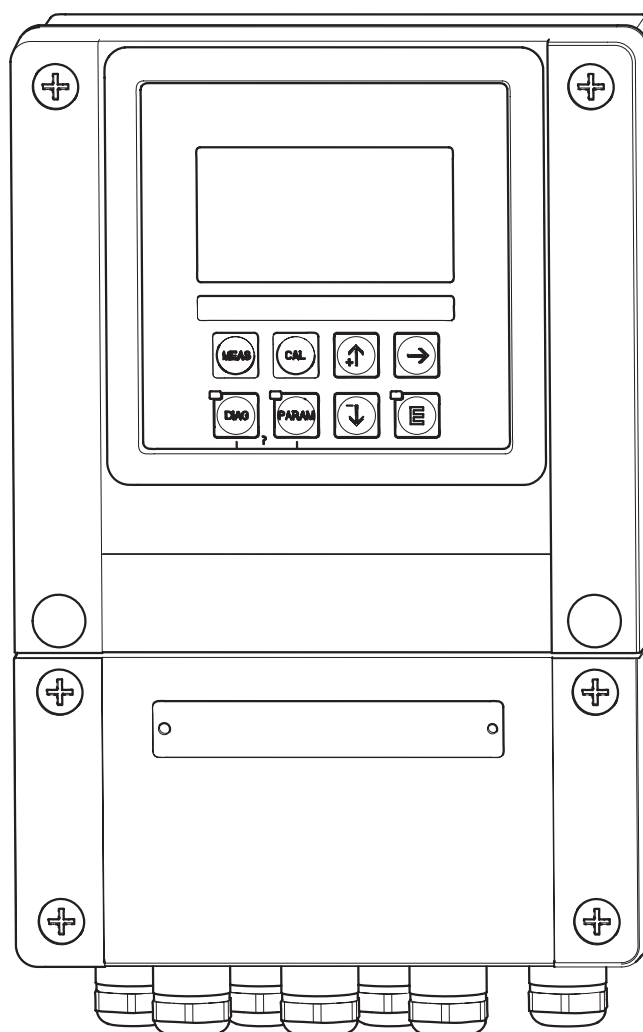

Brief overview

Here is how to use these Operating Instructions to commission your Mycom S quickly and safely:

→ page 5 ff. → page 5	Safety instructions General safety instructions Explanation of the warning symbols You can find special instructions at the appropriate position in the chapter in question. The significance is indicated with the icons ⚠ Warning, ⚡ Caution, 📝 Note.
→ page 10 ff.	Installation Mounting types and the steps for installing the instrument as well as its dimensions can be found here.
→ page 13 ff.	Mycom S wiring On these pages, you can find the required steps for electrical connection of your Mycom S and a complete wiring diagram.
→ page 19 ff.	Display and operating elements Use this chapter to get familiar with the device operation.
→ page 25 ff.	First start up First start up is automatically started when starting the instrument for the first time. It allows you to commission your instrument quickly and easily.
→ page 83 ff.	Calibration Here, you can find the required steps for calibration of transmitter and sensor. Always perform a calibration during first commissioning.
→ page 31 ff.	Customer-specific configuration This chapter explains how to configure additional functions via the software thus adapting the transmitter to your requirements.
→ page 87 ff.	Maintenance Information on maintenance tasks and maintenance intervals can be found here.
→ page 92 ff.	Troubleshooting If faults occur during operation, use the check lists to localise and eliminate the cause.

Table of Contents

1	Safety instructions	5		
1.1	Notes on safety conventions and icons	5		
1.2	Designated use	6		
1.3	Installation, Commissioning, Operation	6		
1.4	Operational safety	7		
1.5	Return	7		
2	Identification	8		
2.1	Device designation	8		
2.1.1	Product structure	8		
2.1.2	Nameplate	9		
2.2	Scope of delivery	9		
2.3	Certificates and approvals	9		
3	Installation	10		
3.1	Incoming acceptance, transport, storage	10		
3.2	Installation conditions	10		
3.2.1	Dimensions	10		
3.3	Installation	10		
3.3.1	Installation instructions	10		
3.3.2	Wall mounting	11		
3.3.3	Post mounting and panel mounting	11		
3.4	Post-installation check	12		
4	Wiring	13		
4.1	Quick wiring guide	13		
4.1.1	Wiring diagram	13		
4.1.2	Connection compartment label	14		
4.2	Connecting the measuring system	15		
4.2.1	Contact assignment	15		
4.2.2	Sensor connection and measuring cable	16		
4.3	Post-connection check	18		
5	Operation	19		
5.1	Display and operating elements	19		
5.1.1	Display reading/symbols	19		
5.1.2	Key assignment	19		
5.1.3	Measuring menus	20		
5.1.4	Data log	21		
5.1.5	Operation access authorisation	21		
5.1.6	Menu editor types	22		
5.2	Replaceable memory	23		
6	Commissioning	24		
6.1	Function check	24		
6.2	Switching on the measuring device	24		
6.3	First start up	25		
6.4	Description of functions	31		
6.4.1	Set up 1 – Sensor input	31		
6.4.2	Set up 1 – Display	34		
6.4.3	Set up 1 – Access codes	35		
6.4.4	Set up 1 – Current outputs	36		
6.4.5	Set up 1 – Relays	40		
6.4.6	Set up 1 – Temperature	42		
6.4.7	Set up 1 – Concentration	46		
6.4.8	Set up 1 – Alarm	48		
6.4.9	Set up 1 – Hold	50		
6.4.10	Set up 1 – Parameter sets	51		
6.4.11	Set up 1 – Emergency switching	54		
6.4.12	Set up 2 – Data log	55		
6.4.13	Set up 2 – Check	56		
6.4.14	Set up 2 – Controller settings	56		
6.4.15	Set up 2 – Limit switch	70		
6.4.16	Set up 2 – Controller quick adjustment	72		
6.4.17	Set up 2 – Chemoclean	73		
6.4.18	Manual operation	78		
6.4.19	Diagnosis	79		
6.4.20	Calibration	83		
7	Maintenance	87		
7.1	Maintaining the measuring system	87		
7.1.1	Cleaning	87		
7.1.2	Inspecting cables and connections	88		
7.1.3	Simulation of conductive sensors for device test	88		
7.1.4	Simulation of inductive sensors for device test	89		
7.1.5	Checking conductive conductivity sensors	90		
7.1.6	Checking inductive conductivity sensors	90		
7.1.7	Checking line extension and boxes	90		
8	Troubleshooting	91		
8.1	Troubleshooting instructions	91		
8.1.1	Error number list: Troubleshooting and configuration	92		
8.1.2	Process-specific errors	95		
8.1.3	Instrument-specific errors	97		
8.2	Response of outputs to errors	98		
8.2.1	Response of current outputs	98		
8.2.2	Response of contacts to errors	98		
8.2.3	Response of contacts to power failure	98		
8.3	Spare parts	98		
8.4	Installation and removal of parts	100		
8.4.1	Instrument view	100		
8.4.2	Coding	101		
8.5	Replacing the device fuses	101		
8.6	Disposal	101		

9	Accessories	102			
10	Technical data	104			
10.1	Input	104			
10.2	Output	105			
10.3	Performance characteristics	107			
10.4	Environment	107			
			10.5	Mechanical construction	108
			11	Appendix	109
			11.1	Operating matrix	109
			12	Index	120

1 Safety instructions

1.1 Notes on safety conventions and icons

General safety instructions



Warning!

This symbol alerts you to hazards which could cause serious injuries as well as damage to the instrument if ignored.



Caution!

This symbol alerts you to possible faults which could arise from incorrect operation. They could cause damage to the instrument if ignored.



Note!

This symbol indicates important items of information.

Electrical symbols



DC voltage

A terminal at which DC voltage is applied or through which DC flows.



AC voltage

A terminal at which (sine-form) AC voltage is applied or through which AC flows.



Ground connection

A grounded terminal, which, from the user's point of view, is already grounded using a ground system.



Protective earth terminal

A terminal which must be grounded before other connections may be set up.




Equipotential connection

A connection which must be connected to the grounding system of the equipment. This can be, for example, a potential matching line of a star-shaped grounding system, depending on national or company practice.



Double insulation

The equipment is protected with double insulation.



Alarm relay



Input



Output

1.2 Designated use

The transmitter Mycom S CLM153 is a device for measuring conductivity. The transmitter is designed for measuring or control tasks in applications in the following industries:

- Chemical process systems
- Pharmaceuticals
- Foodstuff industry
- Water treatment and monitoring

The Ex-version of the Mycom S CLM153 makes operation in hazardous atmospheres also possible (see "Certificates" in the product structure on page 8).

Any other use than the one described here compromises the safety of persons and the entire measuring system and is, therefore, not permitted.

The manufacturer is not liable for damage caused by improper or non-designated use.

1.3 Installation, Commissioning, Operation

Please note the following items:

- Installation, electrical connection, commissioning, operation and maintenance of the measuring system must only be carried out by trained technical personnel.
- The technical personnel must be authorised for the specified activities by the system operator.
- Technical personnel must have read and understood these Operating Instructions and must adhere to them.
- Before commissioning the entire measuring point, check all the connections for correctness. Ensure that electrical cables and hose connections are not damaged.
- Do not operate damaged products and secure them against unintentional commissioning.
- Measuring point faults may only be rectified by authorised and specially trained personnel.
- If faults cannot be rectified, the products must be moved from service and secured against unintentional commissioning.
- Repairs not described in these Operating Instructions may only be carried out at the manufacturer's or by the Endress+Hauser service organisation.

1.4 Operational safety



Warning!

If the device is used for any application other than those described in these Operating Instructions, it may lead to unsafe and improper functioning of the measuring system and is therefore not permitted.

The instrument has been designed and tested according to the state of the art and left the factory in perfect functioning order. The instrument meets all the prevailing regulations and EC directives – see "Technical data".

However, always pay attention to the following points:

- Measuring systems used in Ex areas have a separate document (XA 233C/07/a3) which forms a component part of these Operating Instructions. Always follow the installation regulations and the – partly deviating – connection data of the Ex documentation as well. You can find the following symbols on the front page of the additional Ex documentation (according to approval and test centre (CE Europe,  USA,  Canada).
- The measuring device complies with the general safety requirements in accordance with EN 61010, the EMC requirements of EN 61326, and NAMUR Recommendation NE 21, 1998.
- The manufacturer reserves the right to change the technical data in line with technical progress at any time. You can obtain information on the current version of these Operating Instructions and possible additions from your responsible sales centre.

Immunity to interference

This instrument has been tested for electromagnetic compatibility in industrial use according to applicable European standards. It is protected against electromagnetic interference by the following design measures:

- cable screening
- interference suppression filter
- interference suppression capacitors



Warning!

Protection against interference as specified above is valid only for an instrument connected according to the instructions in these Operating Instructions.

1.5 Return

If the transmitter has to be repaired, please return it cleaned to the sales centre responsible. You can find the address on the last page of these instructions. For returns please use the original packaging. With the instrument, please enclose a completed copy of the "Declaration of Contamination" form. You can find this at the end of these Operating Instructions.

2 Identification

2.1 Device designation

2.1.1 Product structure

Conductivity transmitter in aluminium housing for wall mounting with one alarm and two output contacts for NAMUR, Chemoclean and controller functions as well as three binary inputs, logbooks, data logs, USP limit functions (USP = United States Pharmacopeia). Plain text operation. 247x167x111 mm (HxWxD). Degree of protection IP 65.

Certificates									
A									Basic equipment: non-Ex
G									With Atex approval, Atex II (1) 2G EEx em ib[ia] IIC T4
O									With FM approval; NI Cl. I, Div. 2, Sensor IS Cl. I, Div. 1
P									With FM approval; NI Cl. I, Div. 2
S									With CSA approval; NI Cl. I, Div. 2, Sensor IS Cl. I, Div. 1
T									With TIIS approval
Measuring input									
1									1 measuring circuit for conductive sensors, conductivity/resistivity and temperature
2									1 measuring circuit for inductive sensors, conductivity/resistivity and temperature
3									2 measuring circuits for conductive sensors, conductivity/resistivity and temperature
4									2 measuring circuits for inductive sensors, conductivity/resistivity and temperature
Measuring output									
A									2 current outputs 0/4 ... 20 mA, passive (Ex and non-Ex)
B									2 current outputs 0/4 ... 20 mA, active (non-Ex)
C									HART with 2 current outputs 0/4 ... 20 mA, passive (Ex and non-Ex)
D									HART with 2 current outputs 0/4 ... 20 mA, active (non-Ex)
E									PROFIBUS-PA, without current outputs
Contacts, current input									
0									Without additional contacts
1									3 additional contacts
2									2 additional contacts, 1 passive current input (Ex and non-Ex)
3									2 additional contacts, 1 resistance input (non-Ex)
4									1 additional contact, 2 passive current inputs (Ex and non-Ex)
5									1 additional contact, 1 passive current input, 1 active resistance input (non-Ex)
Power supply									
0									100 ... 230 V AC
8									24 V AC / DC
Language versions									
A									E / D
B									E / F
C									E / I
D									E / ES
E									E / NL
F									E / J
Cable connection									
0									Cable glands M 20 x 1.5
1									Adapter for cable gland NPT ½"
2									Adapter for cable gland G ½"
Additional equipment									
0									Without additional equipment
1									Additional equipment: DAT module
Configuration									
0									Factory settings
CLM153-									Complete order code

2.1.2 Nameplate

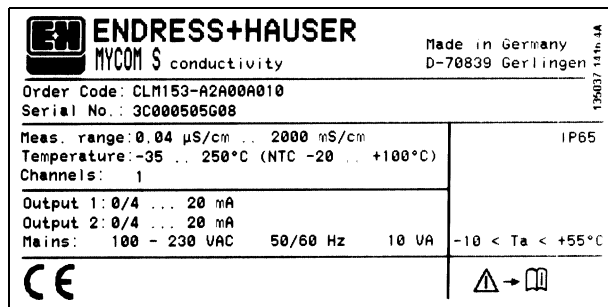


fig. 1: Example of a nameplate for the transmitter Mycom S CLM153.

2.2 Scope of delivery

The scope of delivery comprises:

- 1 transmitter
- 1 mounting kit
- 4 cable glands
- 1 set for measuring point labelling
- 1 instrument identification card
- 1 operating instructions English
- Versions with HART communication:
 - 1 operating instructions Field communication with HART, English
- Versions with PROFIBUS interface:
 - 1 operating instructions Field communication with PROFIBUS PA, English
- Ex versions according to ATEX:
 - Safety instructions for electrical equipment in explosion hazardous areas, XA 233C/07/a3

2.3 Certificates and approvals

Declaration of conformity

The product meets the legal requirements of the harmonised European standards. Endress + Hauser confirms compliance with the standards by affixing the **CE** symbol.

3 Installation

3.1 Incoming acceptance, transport, storage

- Make sure the packaging is undamaged!
Inform the supplier about damage to the packaging.
Keep the damaged packaging until the matter has been settled.
- Make sure the contents are undamaged!
Inform the supplier about damage to the delivery contents.
Keep the damaged products until the matter has been settled.
- Check that the scope of delivery is complete and agrees with your order and the shipping documents.
- The packaging material used to store or transport the product must provide shock protection and humidity protection. The original packaging offers the best protection.
Also, keep to the approved ambient conditions (see "Technical data").
- If you have any questions, please contact your supplier or your sales centre responsible.



Note!

The yellow dummy plugs in the cable glands of Mycom S are only used for transport security. They do not provide IP 65.

3.2 Installation conditions

3.2.1 Dimensions

You can find the dimensions and lengths of the transmitter in the Technical data on page 104 ff.

3.3 Installation

3.3.1 Installation instructions


- The standard use of the Mycom S CLM153 transmitter is as a field instrument.
- The Mycom S CLM153 transmitter can be fixed to vertical or horizontal pipes using the round post fixture available from Endress+Hauser (see Accessories). When installing the instrument outdoors, you also require the weather protection cover CYY 101. This cover is compatible with all field instrument installations options.
- Always install the transmitter so that the cable entries point downwards.
- The transmitter can be installed as a panel-mounted unit as well.

3.3.2 Wall mounting



Caution!

- Check that the temperature does not exceed the maximum permitted ambient temperature ($-20^{\circ} \dots +60^{\circ}\text{C}$ / $-4 \dots +140^{\circ}\text{F}$). Install the instrument in a shady location. Avoid direct sunlight.
- Mount the device so that the cable entries always point downwards.

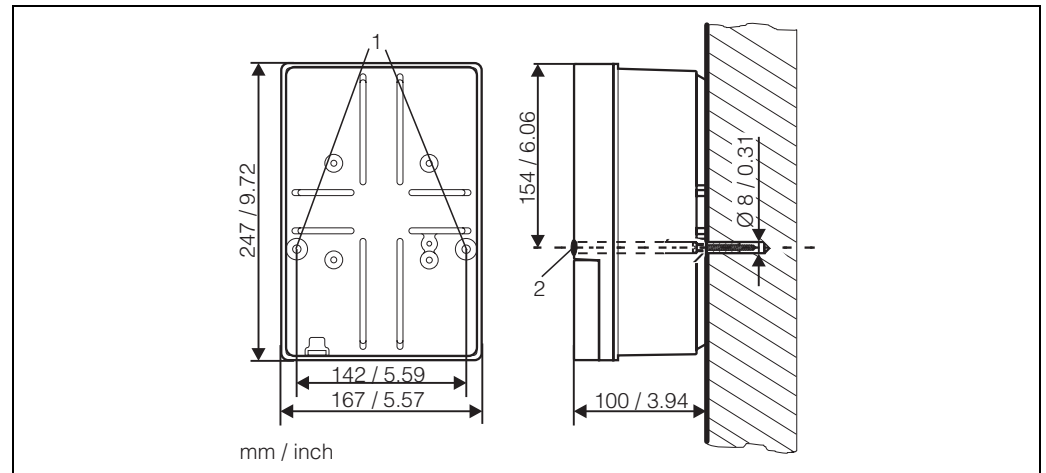


C07-CPM153xx-11-00-08-en.001.eps

fig. 2: Dimensions for wall mounting: Fixing screw: dia. 6 mm / 0.24", Wall plug: dia. 8 mm, 0.31"
1: Fixing drillholes
2: Plastic cover caps

For the wall mounting of the transmitter proceed as follows:

1. Prepare drill holes acc. to fig. 2
2. Push the two fixing screws from the front through the appropriate fixing bores (1).
 - Fixing screws: max. dia. 6.5 mm / 0.26"
 - Screw head: max. dia. 10.5 mm / 0.41"
3. Mount the transmitter housing on the wall as shown.
4. Cover the drill holes with the plastic cover caps (2).

3.3.3 Post mounting and panel mounting

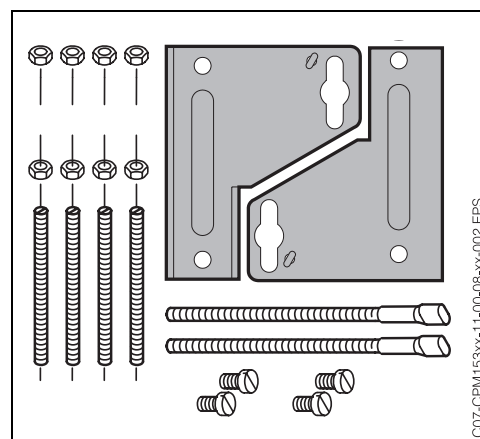


C07-CPM153xx-11-00-08-xx-002.EPS

fig. 3: Mounting kit Mycom S CLM153

Mount the parts of the mounting kit (see accompanying figure) at the back of the housing as depicted in fig. 4.

Required mounting cutout for panel mounting:
161 x 241 mm / 6.34 x 9.49 inches
Installation depth: 134 mm / 5.28
Pipe diameter: max. 70 mm / 2.76"

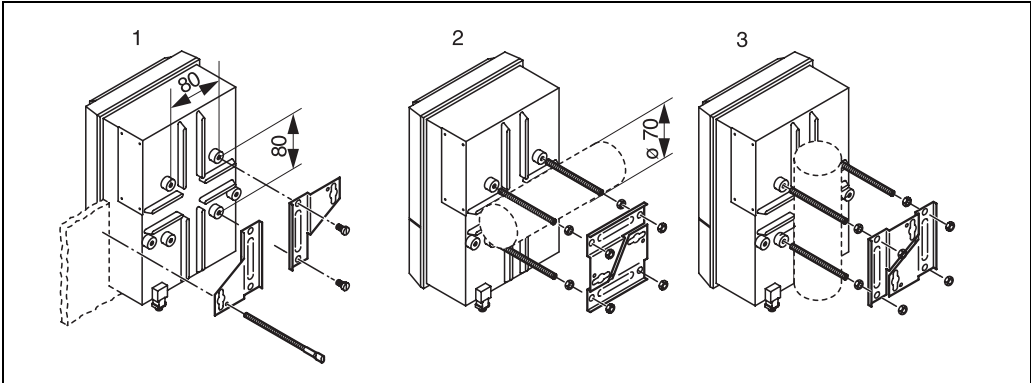


C07-CPM153xx-11-00-08-xx-003.eps

fig. 4: Panel mounting (1) and post mounting for CLM153, horizontal (2) and vertical (3)



Caution!
Danger of device failure. For outdoor use, the weather protection cover CYY 101 is required, (see fig. 5 and Accessories).

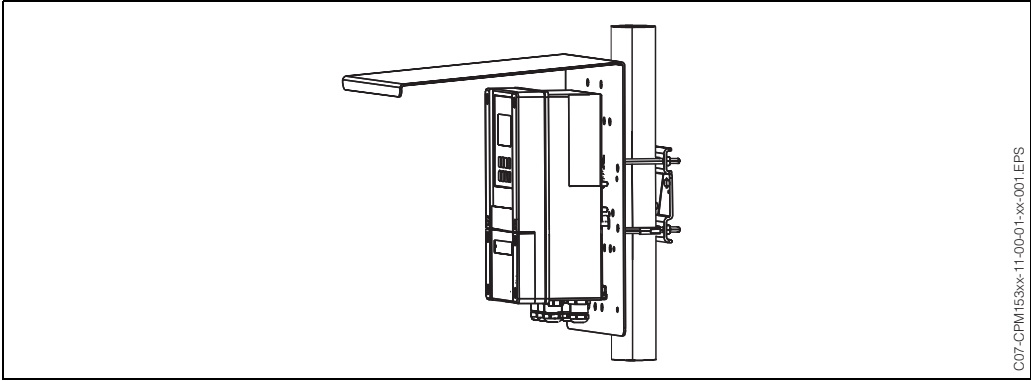

C07-CPM153xx-11-00-01-xx-001.EPS

fig. 5: Post mounting for the transmitter CLM153 with weather protection cover CYY101.

3.4 Post-installation check


After installing the transmitter, carry out the following checks:

Instrument status and specifications	Note
Is the transmitter undamaged?	Visual inspection
Installation	Note
Are the measuring point number and the labelling correct?	Visual inspection
Process environment/conditions	Note
Is the transmitter protected against rainfall and direct sunlight?	For outdoor installation, the weather protection cover CYY101 is required (see Accessories).

4 Wiring

4.1 Quick wiring guide

4.1.1 Wiring diagram

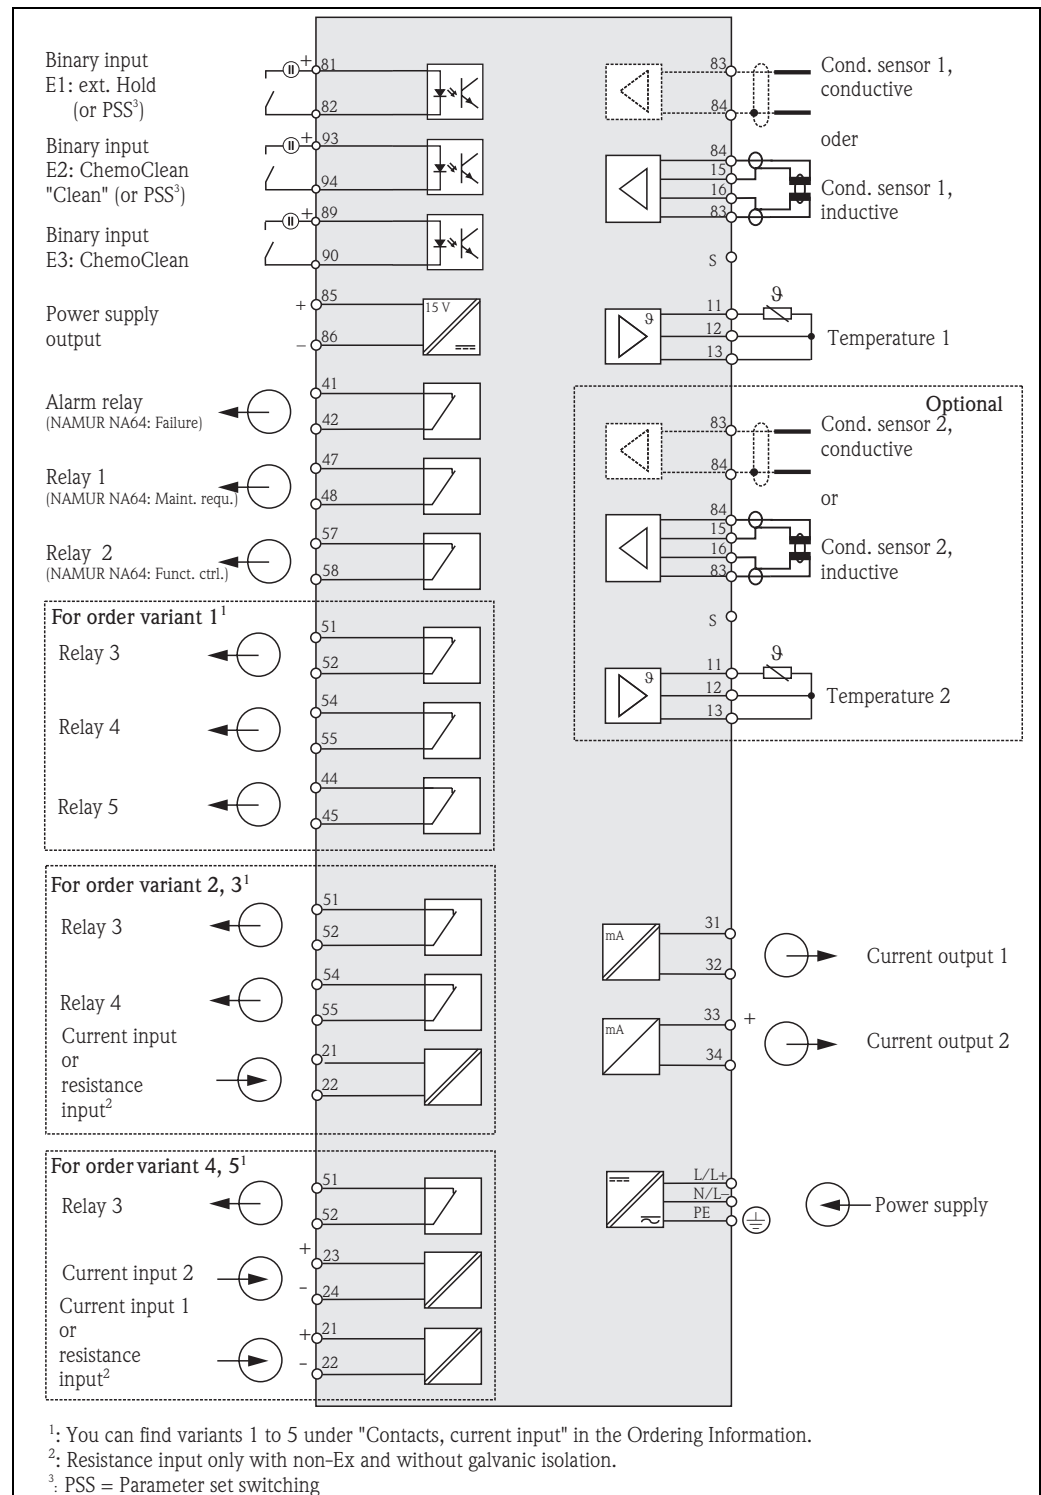

C07-CLM153xx-04-06-00-en-001.eps

fig. 6: Electrical connection CLM153



Warning!
A mains disconnecting device must be installed near the instrument and must be identified as the mains disconnection device for the Mycom S CLM153 (see EN 61010-1).



Note!
■ Connect unused signal wires from input and output lines to the internal PE rail of the CLM153.
■ The current/resistance input may only be connected using a screened cable, whereby the screen at the transmitter must be applied to the PE rail.

4.1.2 Connection compartment label

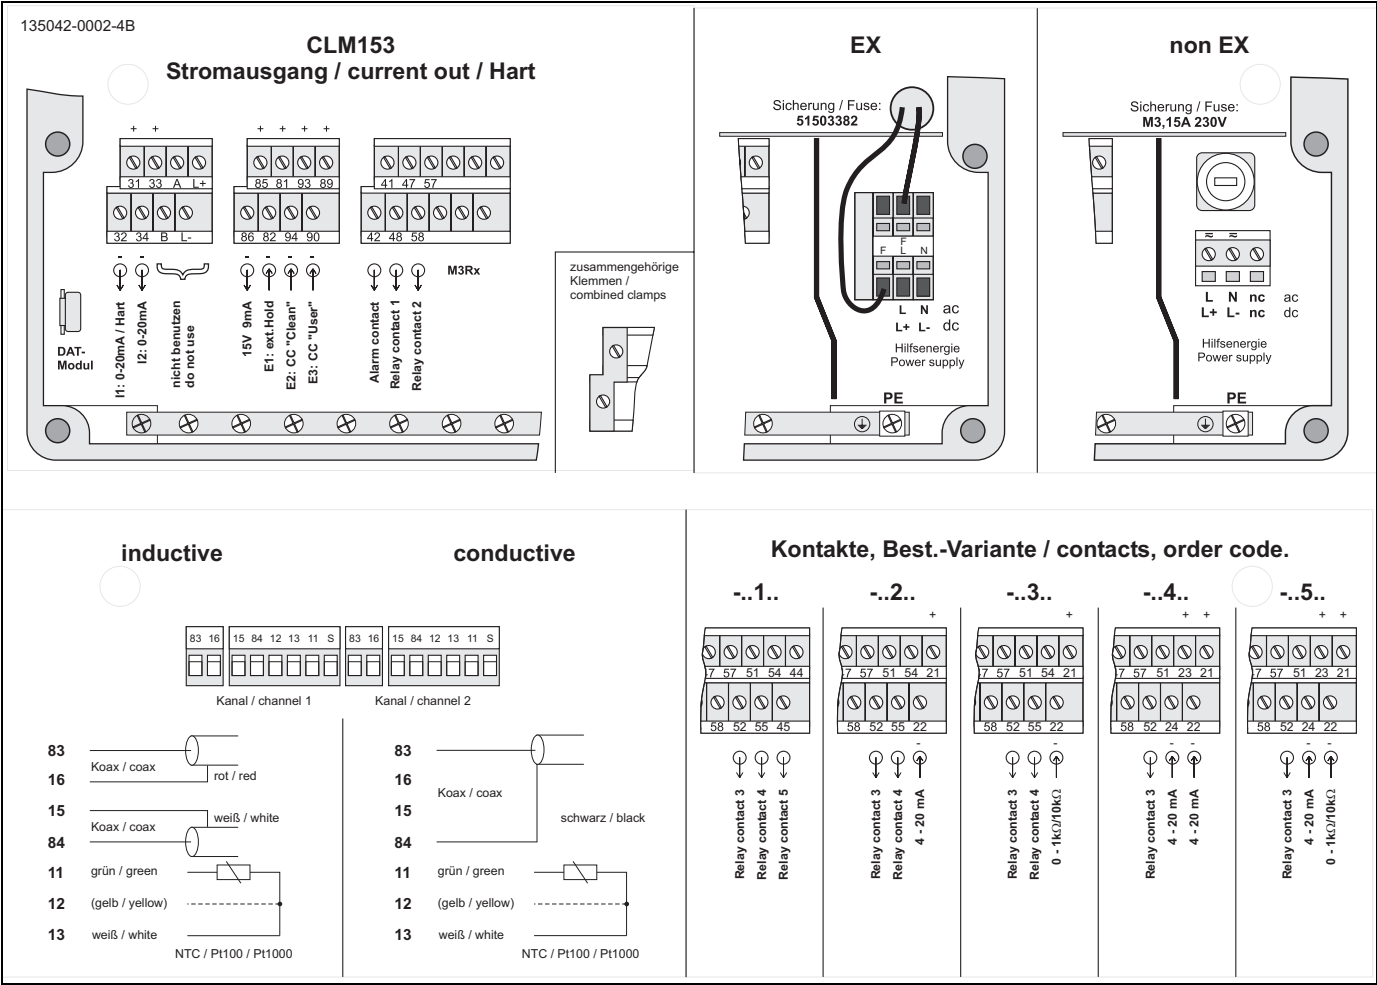


fig. 7: Connection compartment label (in the connection compartment of the transmitter)

4.2 Connecting the measuring system

Connections in the housing cover

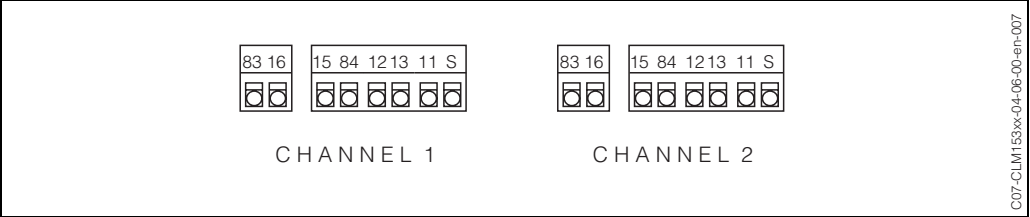


fig. 8: Terminal arrangement in the housing cover of the transmitter

Connections in the lower housing section

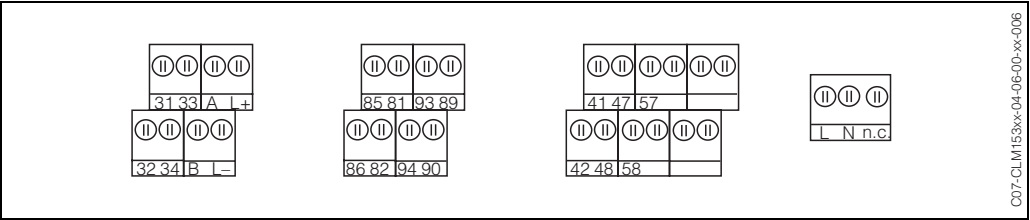


fig. 9: Terminal arrangement in the lower housing section of the transmitter

4.2.1 Contact assignment

In the basic version, the Mycom S CLM153 possesses 1 alarm contact and 2 additional contacts. The instrument can be upgraded with the following **additional** equipment:

- 3 contacts
- 2 contacts and 1 current or resistance input (only for non-Ex)
- 1 contact, 2 current inputs or
- 1 contact, 1 current and 1 resistance input (only for non-Ex)

The available contacts can be assigned via the software (see the menu "PARAM" → "Set up 1" → "Relays" from page 40).



Note!

- If you use NAMUR contacts acc. to working sheet NA64, the contacts are set to the relays as follows:
 - "Failure" to ALARM
 - "Maintenance required" to RELAY 1 and
 - "Function check" to "RELAY 2".

Selection by software	NAMUR on	NAMUR off
ALARM 	Failure	Alarm
RELAY 1 	Warning when maintenance required	freely selectable
RELAY 2 	Function check	freely selectable


- You can assign up to three relays to the controllers.

4.2.2 Sensor connection and measuring cable

Cable types


You require screened special cables to connect conductivity sensors.
You can use the following multicore and preterminated cable types:

- CYK71 for conductive conductivity sensors (CYK71-Ex for Ex applications)
- CPK9 with TOP68 plug-in head for conductive conductivity sensors with and without integrated temperature sensor (for high-temperature applications, IP 68 / NEMA 6X, also for Ex).
- CLK5 for inductive conductivity sensors.

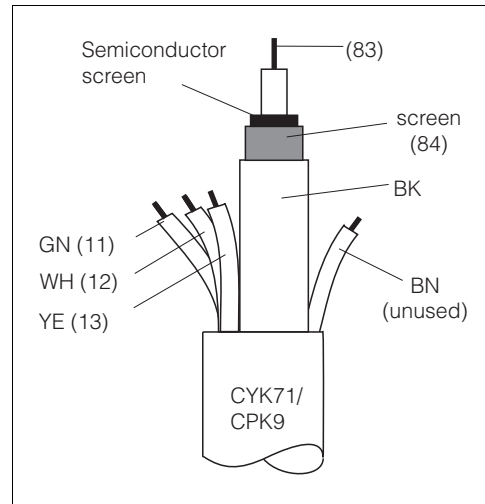

C07-CYK71xxx-00-11-00-en-003.eps


fig. 10: Design measuring cable CYK71 or CPK9

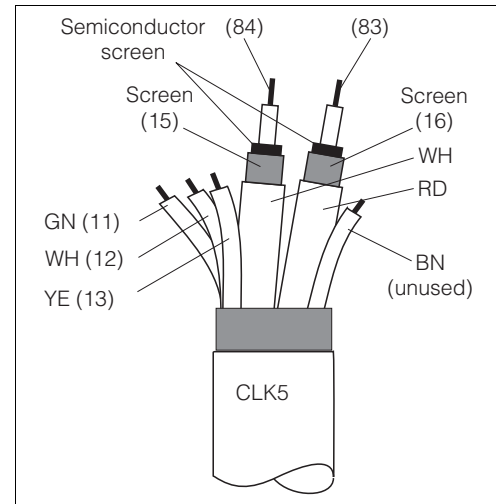

C07-CLK5xxxx-00-05-00-en-002.eps


fig. 11: Design measuring cable CLK5

Connection examples

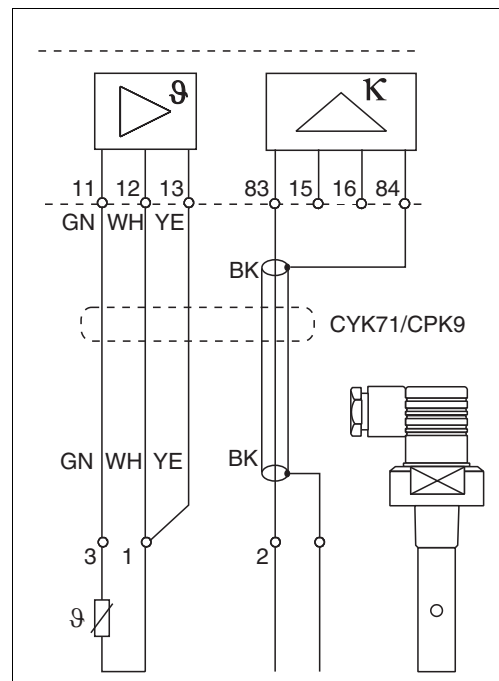

C07-CLM153xx-04-06-00-xx-002.eps

fig. 12: Connection of conductive sensors (CLS15, CLS19, CLS20, CLS21)

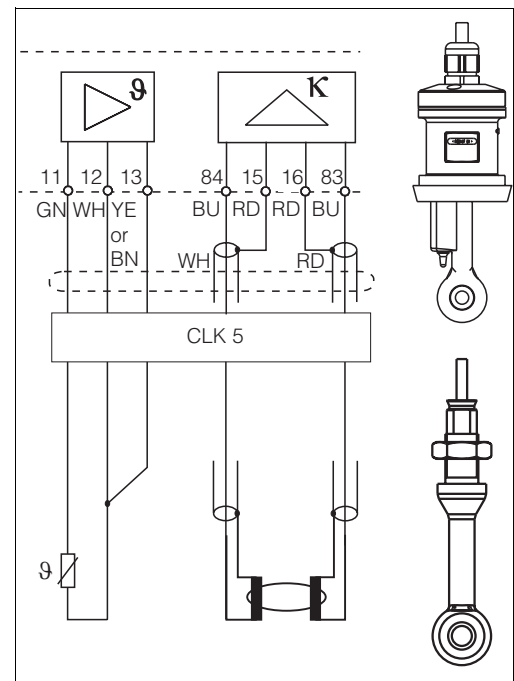

C07-CLM153xx-04-06-00-xx-003.eps

fig. 13: Connection of inductive sensors (CLS50, CLS52)

Outer screen connection

The outer cable screen is electrically connected to the housing via the metall cable gland.



Caution!
Danger of inaccuracy.
Always protect plugs, terminals and cables against humidity.

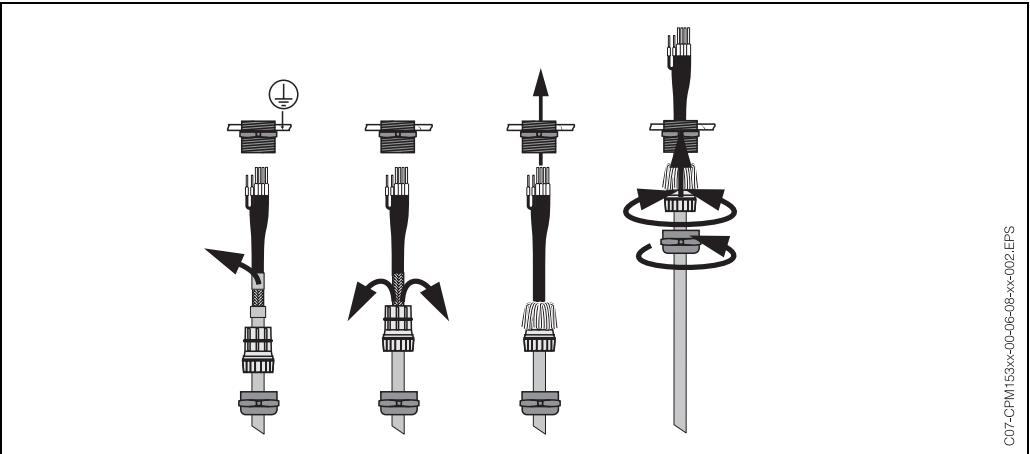


fig. 14: Outer screen connection for CPK9 for example with metal cable gland.
The screen contact is within the cable gland.

Cable extension

If a cable extension is necessary, use

- junction box VBM or VBM-Ex

and the following types of non-terminated measuring cables:


- for CPK9: cable CYK71 or CYK71-Ex
- for CLK5: cable CLK5

Maximum cable length

Conductivity measurement, conductive	Conductivity measurement, inductive
max. 100 m / 328.10 ft with CYK71 (corresp. 10 nF). When $k=1$, you should reckon with reduced accuracy in the range 200 mS/cm at line resistances $> 5 \Omega$ (5 Ω corresponds to approx. 20 m / 65.62 ft CYK cable). If necessary, use a cable with a larger cross-section.	Max. 55 m / 180.46 ft (with CLK5 and sensor cable)
Max. cable length for resistivity measurement: 15 m / 49.22 ft	

Note!

With all cable types, the inner coaxial cable has a black, plastic, semi-conductor layer (arrow), which you must remove.

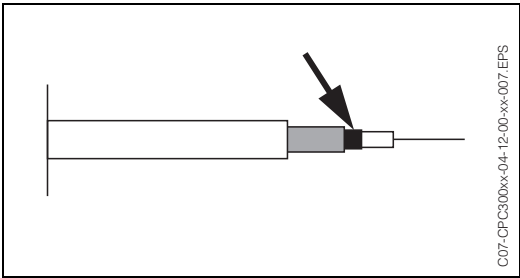

4.3 Post-connection check


After wiring up the electrical connection of the measuring instrument, carry out the following checks:

Instrument status and specifications	Note
Is the measuring instrument or the cable damaged externally?	Visual inspection
Electrical connection	Note
Does the supply voltage match the specifications on the nameplate?	100 V ... 230 V AC long-range 24 V AC / DC
Do the cables used fulfil the required specifications?	Use a genuine E+H cable for sensor and sensor connection, see Accessories chapter.
Are current/resistance inputs connected screened?	
Are the mounted cables strain-relieved?	
Is the cable type route completely isolated?	Along the whole cable length, run the power supply and signal line cables separately to avoid any mutual influence. Cable channels are best.
No loops and cross-overs in the cable run?	
Are the power supply and signal cable correctly connected according to the wiring diagram?	
Are all the screw terminals tightened?	
Are all the cable entries installed, tightened and sealed? Cable run with "water sag"?	"Water sag": cable circuit hanging down so that water can drip off.
Are all the housing covers installed and tightened?	Check seals for damage.

5 Operation

5.1 Display and operating elements

5.1.1 Display reading/symbols

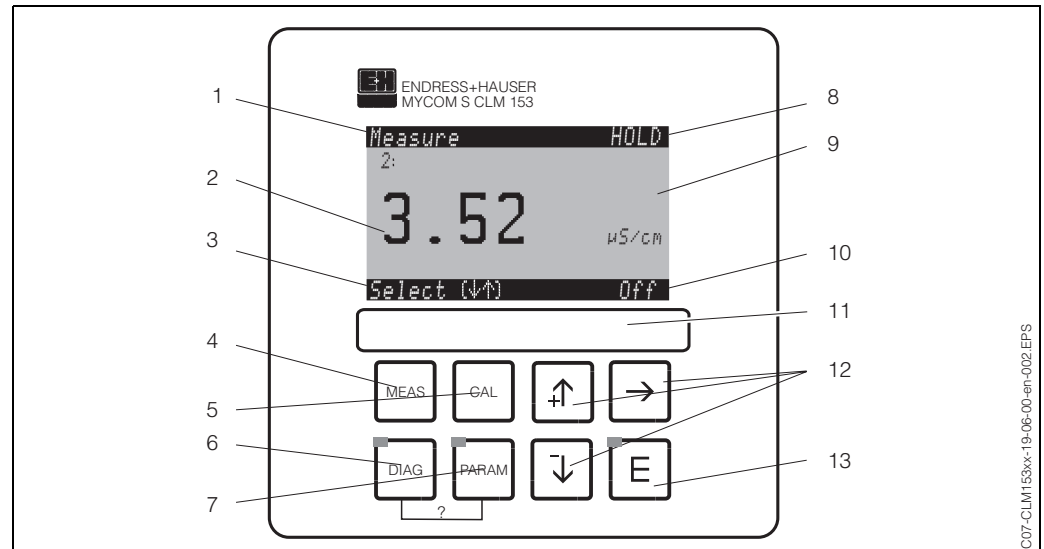

Mycom S CLM153 user interface

1: Current menu

2: Current parameter

3: Navigation bar: Arrow keys for scrolling, "E" for browsing, note for Cancel

4: "Meas" (Measuring mode) key

5: "CAL" (Calibration) key

6: "DIAG" (Diagnosis menu) key

7: "PARAM" (Parameter entry menu) key

? = Press DIAG and PARAM simultaneously to open the help pages

8: HOLD display, if HOLD active; PS1 = parameter set 1

9: Current primary measured value

10: "Failure" display, "Warning", if the NAMUR contacts respond

11: Labelling strip

12: Arrow keys for scrolling and editing

13: Enter key

5.1.2 Key assignment



"PARAM" brings you to the menu for configuring the Mycom S CLM153.

Note!


"PARAM" allows you to return to the previous "return field" from any point in the menu. These are marked in bold in the menu overview (s. chap. 11.1).

LED: This is the send LED for the service adapter "Optoscope" (see "Accessories").

Brings you to the instrument diagnosis menu.



LED: This is the receive LED for the service adapter "Optoscope" (see "Accessories").



Help:

Press the "DIAG" and "PARAM" keys simultaneously to open the help page.



"MEAS" switches to Measuring mode. This displays the measured values. Use the arrow keys to scroll through the different measuring menus.

Note!

Press "MEAS" to exit any of the "PARAM", "DIAG", "CAL" menus without terminating the settings / calibration.



"CAL" switches to the calibration menu for calibrating the sensors.




"E" (Enter) moves you one step forward in a menu or confirms a selection you made.

LED (status display)

Green: everything OK.

Red: an error has occurred.



- You can scroll through the items with the arrow keys, and then highlight your selection (if there is a choice offered)
or
- Increment or decrement numbers by one step with "+" / "-".
Move to the next digit with the "right arrow" (editor type 1) or
- "Activate" with the "right arrow" and scroll through the selection with "+" / "-"
(editor type 2) (for information on editor types, see page 22).

5.1.3 Measuring menus

You can choose between the different measuring menus. Use the arrow keys to scroll between the different menus.

Two-circuit: Both primary values are displayed.		One-circuit: The current measured value is displayed. Two-circuit: The current measured value of circuit 1 or 2 is displayed.		One-circuit/Two-circuit: If you have activated one (both) data logger, you can see the current measured value(s) characteristic here in the record mode (subsequently).		Two-circuit: With a two-circuit device and combined circuits you can display a selected characteristic value and the temperatures of both circuits.	
Two-circuit: The combined value and both single values are displayed.		Two-circuit: With a two-circuit device, in this measuring menu you can see both measured values next to each other and their corresponding temperatures.		In this measuring menu, you can see the current and voltage values and the contact states of the relay at a glance (one-circuit device: only primary value 1). Active relay = ☒ (with function) Inactive relay = ☐		One-circuit: With a one-circuit device you can see the primary value (temperature compensated and below non-temperature compensated) with the corresponding temperature.	

5.1.4 Data log


In the CLM153, you have two data logs available. With these data logs you can

- record a parameter with 500 sequential measuring points or
- two parameters each with 500 sequential measuring points.

To be able to use the function, activate the data logger(s) in the "PARAM" menu → "Set up 2" → "Data Log" (s. page 55). The function is active immediately.

You can view the measured values by scrolling through the different measuring menus (see above).

- The current measured values are recorded in Record mode.
- In Scroll mode, you can open saved data with date and time. To display data, select "PARAM" → "Set up 2" → "Data log".

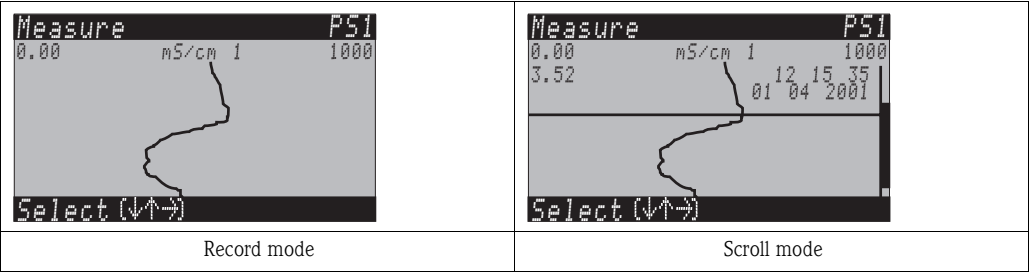

5.1.5 Operation access authorisation

To protect the transmitter against an unintended or undesired change in the configuration and calibration data, functions can be protected using four-digit access codes.

Access authorisation has the following levels:

Read-only level (accessible without a code):

The complete menu can be viewed. The configuration cannot be altered. No calibration is possible. On this level, only the control parameters for new processes can be changed in the "DIAG" menu branch.

Maintenance code

Maintenance level (can be protected by the maintenance code):

This code allows access to the calibration menu.

Use this code to operate the temperature compensation item. The factory functions and the internal data can be viewed.

Factory setting Code = 0000, i.e. the levels are not protected.

In case you have mislaid/forgotten the supplied maintenance code, contact your Endress+Hauser service.

Specialist code

Specialist level (can be protected by the specialist code):

All menus can be accessed and changed.

Factory setting Code = 0000, i.e. the levels are not protected.

In case you have mislaid/forgotten the supplied specialist code, contact your Endress+Hauser service.


To activate the codes (= functions locked) see the item "PARAM" → "Set up 1" → "Access codes" (s. page 35). Enter your desired codes here. If the code is activated, you can only edit the protected areas with the rights mentioned above.



Note!

- Note down the selected code as well as the universal code and keep it in a place where unauthorised persons do not have access to it.
- If you reset the code to "0000", all the levels are freely accessible again for editing. The code can only be reset by a "specialist".


Locking the operation



This key combination locks the instrument from in-field configuration operations. To lock it, press "CAL" and "DIAG" simultaneously.

At the code prompt, the code appears as "9999". Only the settings in the "PARAM" menu can be seen.

Unlocking the operation



Press the "MEAS" and "PARAM" keys simultaneously to unlock the operation.


5.1.6 Menu editor types

At parameter setting, the functions can be selected in two different modes, depending on the setting type.

Editor type E1

Editor type 1 (E1)

for functions, which can be directly selected from the display. The editing row shows "Edit".

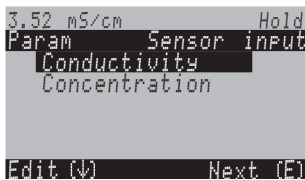


- A selection can be highlighted with the arrow keys.
- Confirm the selection by pressing "E" (=Enter).

Editor type E2

Editor type 2 (E2)

for settings, which have to be defined more precisely, e.g. day, time. The editing row shows "Select".

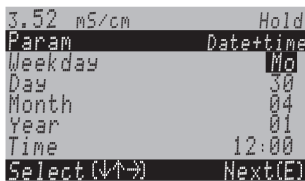

- Use the arrow keys  and  to highlight a selection (e.g. "Mo").
- Activate the selected option with the right arrow key . The highlighted option flashes.
- Scroll through the selection (e.g. the weekdays) with the arrow keys  and .
- Confirm the selection by pressing "E" (=Enter).
- If you make your selection and confirm it by pressing "E" (no flashing display), you can exit the item by pressing "E".

5.2 Replaceable memory

The DAT module is a memory device (EEPROM) which is plugged into the connection compartment of the transmitter. Using the DAT module you can

- save the complete settings, the logbooks and the data log of a transmitter and
- copy the complete settings to other CLM153 transmitters with identical hardware functionality.

This considerably reduces the effort to install or service several measuring points.

6 Commissioning

6.1 Function check

**Warning!**

Before power-up, make sure there is no danger to the measuring point. Uncontrolled actuated pumps, valves or similar could lead to damage to instruments.

**Caution!**

- Before switching on, check all the connections again for correctness.
- Make sure that the conductivity sensor and, if necessary, the temperature sensor are in the medium or in a calibration solution, as otherwise no plausible measured value can be displayed.
- Also, make sure that the post-connection check has been carried out (s. chap. 4.3).

6.2 Switching on the measuring device

Before first start-up, make sure you understand how to operate the transmitter. You should make particular reference to chapters 1 (Safety instructions) and 5 (Operation).

First commissioning

On first switch-on, the instrument starts automatically with the First start up menu. This asks you about the most important instrument settings. After you close the menu, the instrument is ready for use and measurement in its standard configuration.

**Note!**


- You must completely run through the Quick Setup menu. If you do not, the instrument will not be operational. If you interrupt Quick Setup, it will start again the next time you start it up until **all** the items have been processed and completed.
- For parameter setting, you have to enter the specialist code (default setting 0000).




6.3 First start up




In this menu, configure the most important transmitter functions required for measurement.





The First start up ist started automatically when starting the instrument. You can open it at any time from the menu structure.






To enter the menu, proceed as follows:

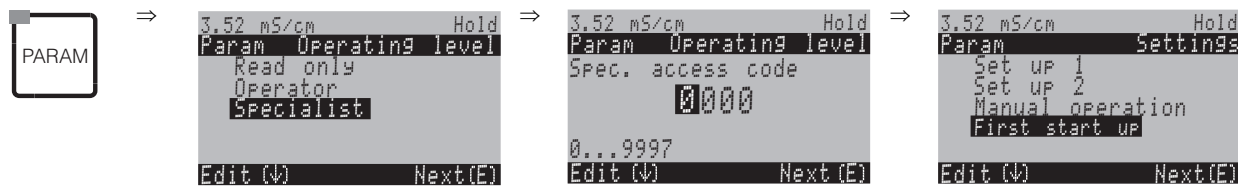

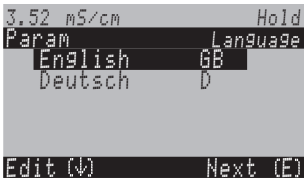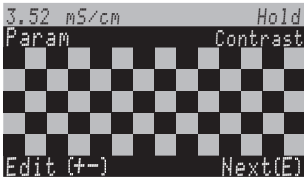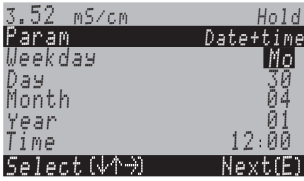
CODE	DISPLAY	CHOICE (default = bold)	INFO
T1		E D	Select language Depending on ordered language version. Language versions: Version -A: E / D Version -B: E / F Version -C: E / I Version -D: E / ES Version -E: E / NL Version -F: E / J
T2			Contrast setting You can increase and reduce the contrast with the +/- keys.
T3		Mo 01 04 01 12:00	Entry of date and time Enter the complete date and time here.

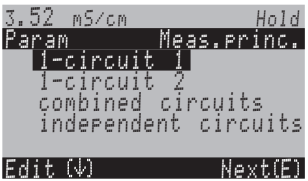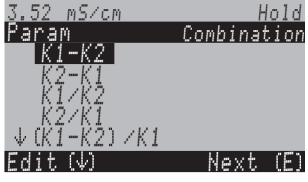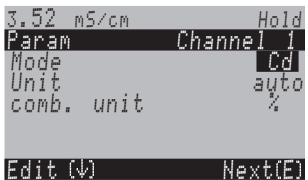CODE	DISPLAY	CHOICE (default = bold)	INFO
T4		One circuit input 1 One circuit input 2 Combined circuits Independent circuits Comb. circuits look-ahead Ind. circuits look-ahead	Select measuring principle (only for two-circuit device) One circuit input 1 / input 2 = measurement via sensor input 1 or 2 Combined circuits = measurement via both sensor inputs with the option of creating a characteristic value (see next field) Independent circuits = independent measurement via both sensor inputs Combined / Independent circuits look-ahead = look-ahead control with combined / independent circuits measurement (only for instruments with 2 current outputs)  Note! ■ If a two-circuit device is configured as such, it keeps these settings even if a transmitter (circuit) is removed or is defective. ■ If, with a defective transmitter, the error message E006, E007 is not required, then you can switch the device to "one circuit". As each relay is assigned to a circuit (alarm, rel. 1, rel. 2 to input 1; rel. 3, 4, 5 to input 2), you should keep in mind that, in such a case, functions which access the deactivated relay are no longer functional.
T5		CH1 – CH2 CH2 – CH1 CH1/CH2 CH2/CH1 (CH1 – CH2)/CH1 (CH2 – CH1)/CH1 (CH1 – CH2)/CH2 (CH2 – CH1)/CH2 pH (CH1 – CH2; VGB)	Select characteristic value (only combined circuits) Here, you can define a process-related characteristic value as a further output parameter.  Note! For determination of the pH value, see chap. 6.4.1, page 31.
T5		Mode: Cd. Unit/medium auto Comb. unit %	Select operating mode (only combined circuits) If the operating mode changes, the user settings are automatically reset. The settings you make here apply to both measuring circuits. Mode: Cd. (conductivity), resistivity (with conductive sensors), concentration (with inductive sensors) Unit (with Cond. operating mode, difference calculation): auto, $\mu\text{S}/\text{cm}$, mS/cm , S/cm , $\mu\text{S}/\text{m}$, mS/m , S/m Unit (with resistivity operating mode, difference calculation): auto, $\text{k}\Omega\cdot\text{cm}$, $\text{M}\Omega\cdot\text{cm}$, $\text{k}\Omega\cdot\text{m}$. The optimum unit is automatically selected with "auto".  Note! If pH is used as combined unit, Cd. mode is preset. Medium (with "concentration" operating mode): NaOH, HNO ₃ , H ₃ PO ₄ , H ₂ SO ₄ , Table 1 to 4 Unit with concentration operating mode: %, for customer specific tables. see Chp. 6.4.7 Comb. unit (with ratio calculation): Unit of the characteristic value defined in the previous field Options: none, % or pH value (conductive sensors only)

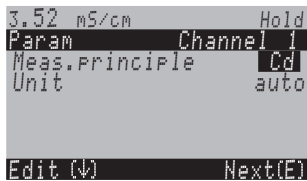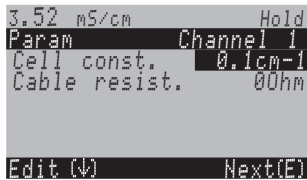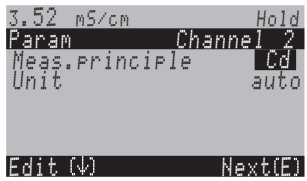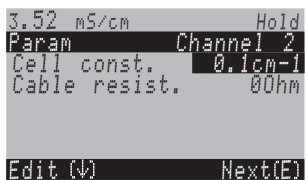CODE	DISPLAY	CHOICE (default = bold)	INFO
T6		Mode Cond. Unit/medium auto	Select the operating mode measuring circuit 1 (not for combined circuits) If the operating mode changes, the user settings are automatically reset. Mode: Cd. (conductivity), resistivity (with conductive sensors), concentration (with inductive sensors) Unit (with Cond. operating mode, difference calculation): auto, $\mu\text{S}/\text{cm}$, mS/cm , S/cm , $\mu\text{S}/\text{m}$, mS/m , S/m Unit (with resistivity operating mode, difference calculation): auto, $\text{k}\Omega\cdot\text{cm}$, $\text{M}\Omega\cdot\text{cm}$, $\text{k}\Omega\cdot\text{m}$. The optimum unit is automatically selected with "auto". Medium (with "concentration" operating mode): NaOH, HNO ₃ , H ₃ PO ₄ , H ₂ SO ₄ , Table 1 to 4 Unit with concentration operating mode: %, for customer specific tables. see Chp. 6.4.7
T7		inductive: Cell const.: 1.98cm-1 Install.factor 1 conductive: Cell const.: 0.1cm-1 Cable resist. 0Ω	Select measuring circuit 1 Cell constant: The exact cell constant is provided in the sensor quality certificate. Cable resistance (for conductive): Enter the cable resistance. Installation factor (only inductive): Enter the installation factor here.
T8		Mode: Cond. Unit/medium auto	Select the operating mode for measuring circuit 2 (not for combined circuits; only two circuit) If the operating mode changes, the user settings are automatically reset. Mode: Cond. (conductivity), resistivity (with conductive sensors), concentration (with inductive sensors) Unit (with Cond. / resistivity operating mode): auto, $\mu\text{S}/\text{cm}$, mS/cm , S/cm , $\mu\text{S}/\text{m}$, mS/m , S/m / auto, $\text{k}\Omega\cdot\text{cm}$, $\text{M}\Omega\cdot\text{cm}$, $\text{k}\Omega\cdot\text{m}$. The optimum unit is automatically selected with "auto". Medium (with "concentration" operating mode): NaOH, HNO ₃ , H ₃ PO ₄ , H ₂ SO ₄ , Table 1 to 4 Unit with concentration operating mode: %, for customer specific tables. see Chp. 6.4.7
T9		inductive: Cell const.: 1.98cm-1 Install.factor 1 conductive: Cell const.: 0.1cm-1 Cable resist. 0Ω	Select measuring circuit 2 (only two circuit) Cell constant: The exact cell constant is provided in the sensor quality certificate. Cable resistance (for conductive): Enter the cable resistance. Installation factor (only inductive): Enter the installation factor here.
T10		°C °F	Select temperature unit °C: Degrees Celsius °F: Degrees Fahrenheit

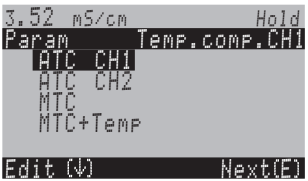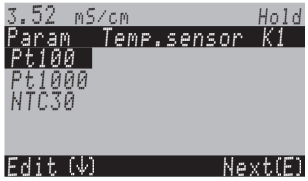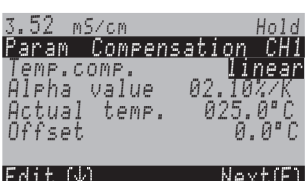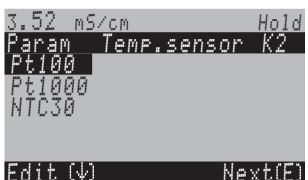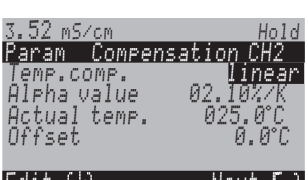CODE	DISPLAY	CHOICE (default = bold)	INFO
T11		ATC CH1 ATC CH2 MTC MTC+Temp	Select temperature compensation channel 1 ATC: Automatic temperature compensation via temperature sensor MTC: Temperature compensation via manual value entry MTC+Temp: Temperature compensation via manual temperature entry. The displayed temperature, however, is measured by the temperature sensor.
T12		Pt 100 Pt 1000 NTC 30k	Select temperature sensor channel1
T13		Temp.comp. linear Alpha value: 2.1%/K Actual temp.: 25.0°C Offset: 0.0°C	Temperature compensation input 1 Temp. comp.: Selection of the temperature compensation – none, linear, NaCl, Table 1 to 4 ultrapure water NaCl (conductive sensors) ultrapure water HCl (conductive sensors) Alpha value: Entry of the conductivity coefficient α (with linear compensation) Actual temp.: The measured temperature is displayed. Offset: Temperature difference between measured and output temperature (–10 ... +10 °C).
T14		ATC CH1 ATC CH2 MTC MTC+Temp	Select temperature compensation channel 2 (only two circuit)
T15		Pt 100 Pt 1000 NTC 30k	Select temperature sensor input 2 (only two circuit)
T16		Temp.comp. linear Alpha value: 2.1%/K Actual temp.: 25.0°C Offset: 0.0°C	Temperature compensation input 2 (only two circuit) Temp. comp.: Selection of the temperature compensation – none, linear, NaCl, Table 1 to 4 ultrapure water NaCl (conductive sensors) ultrapure water HCl (conductive sensors) Alpha value: Entry of the conductivity coefficient α (with linear compensation). Actual temp.: The measured temperature is displayed. Offset: Temperature difference between measured and output temperature (–10 ... +10 °C).

CODE	DISPLAY	CHOICE (default = bold)	INFO
T17	<pre> 3.52 mS/cm Hold Param Relay funct. Acc.Namur off Relais 1 free Relais 2 free Select(↓↑→) Next(E) </pre>	NAMUR off Relay 1: no Relay 2: no	Contact functions Depending on the equipment available, you can assign the function of up to 5 relays here. When you switch on the status message acc. to NAMUR NA64, relays 1 and 2 are assigned and are not available for another function, (compare page 15). Selection: No / Controller / Limit / CCW / CCC Controller: Controller control using relay Limit: Limit switch function CCW: Chemoclean water. Water supply for the Chemoclean function. CCC: Chemoclean Cleaner. Cleaner supply for the Chemoclean function. (Together, CCC and CCW form the "Chemoclean" function. You can find information on Chemoclean on page 73)  Note! If you want to use the USP function, select the limit contactor function for a relay and configure this in the limit value menu for USP (p. 70).
T18	<pre> 3.52 mS/cm Hold Param Current out 1 PV CH1 PV CH2 Temp. CH1 Temp. CH2 Combined Edit (↓) Next (E) </pre>	PV CH1 PV CH2 Temp. CH1 Temp. CH2 Combined	Select the measured value which should be output at the current output 1. Selection possibilities related to the instrument variant and the selected output. PV 1/2: Selection of the primary measured value which you selected, (conduct., conc., resist.) Temperature 1/2: Selection of the temperature to be output to the current output. Combined (only for combined circuits): The characteristic value from Field T5 is output at the current output. Continuous controller (only at current output 2!): Controller output
T19	<pre> 3.52 mS/cm Hold Param Current out 2 PV CH1 PV CH2 Temp. CH1 Temp. CH2 Combined Edit (↓) Next (E) </pre>	PV CH1 PV CH2 Temp. CH1 Temp. CH2 Combined Continuous controller (only at current output 2)	Select measured value which should be output at the current output 2. Selection possibilities see above, Continuous controller (only at current output 2!): The controller actuating variable is output via the current output (see also Controller menu page 56).  Note! Danger of data loss. If you change the assignment for the current output from "continuous controller" to a different function after you have configured the controllers, the entire controller configuration (s. page 56) is reset to the default values.

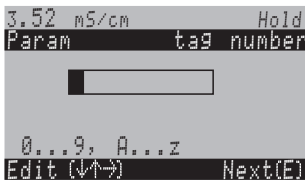CODE	DISPLAY	CHOICE (default = bold)	INFO
T20		(0 ... 9; A ... Z)	Enter your customer specific instrument number. 32-digit tag number. This is saved in the DAT module which is obtainable as an option.
T21		restart end	Exit First start up? restart = Run through settings in Fields T1-T22 again end = Save the settings in Fields T1-T22 and exit First start up.

6.4 Description of functions

6.4.1 Set up 1 – Sensor input

In this menu, you can change the measured value acquisition settings, such as the operating mode, the measuring principle, or the electrode type.

Apart from the measured value attenuation, you have already made all the settings in the menu at the first commissioning in the First start up (s. page 24). You can change the selected values in this menu.

Determination of pH value by differential conductivity (power plants)

When using transmitters for two conductive sensors, the pH value can be selected as characteristic value of combined circuits. It is determined from the difference in conductivity before and after a cation exchanger according to the VGB-R 450L guideline of the Vereinigung der Großkraftwerksbetreiber e.V., Association of Power and Heat Generating Utilities (annex).

Field of application:

Determination of the pH value and the cation conductivity (acid conductivity) in boiler feed water

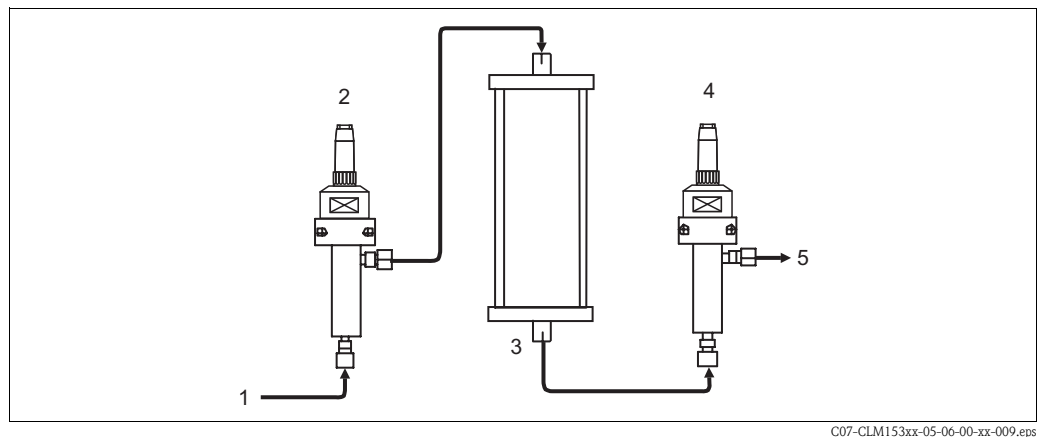


fig. 15: Measuring system for determination of pH value by differential conductivity

- 1 Medium coming from cooler / pressure reducer
- 2 Conductive conductivity sensor (κ_{direct} K1)
- 3 Cation exchanger ($\text{NaCl} \rightleftharpoons \text{HCl}$)
- 4 Conductive conductivity sensor (κ_{acid} K2)
- 5 Outlet

Calculation method according to VGB-R 450L:

$$\text{pH} = 8,60 + \log (\kappa_{\text{direct}} - 1/3 \kappa_{\text{acid}})$$

where

- κ_{direct} (sensor at K1) = conductivity before the cation exchanger (direct conductivity) in $\mu\text{S}/\text{cm}$
- κ_{acid} (sensor at K2) = conductivity after the cation exchanger (acid conductivity) in $\mu\text{S}/\text{cm}$


Conditions:

- The calculation method according to VGB-R 450L presupposes an alkaline operation of the boiler feed water circuit (conditioning with NaOH or NH_3).
- Impurities are mainly NaCl (almost no phosphates: $<0,5 \text{ mg/l}$)
- At pH values < 8 , the impurity concentration must be low compared to the alkaline agent.

**Note!**

- The HCl ultrapure water compensation is used as temperature compensation in both channels.
- Maximum measuring range: pH = 7.0 to 11.0
- When applying a new cation exchanger, correct measured values are only displayed after the exchanger has been rinsed thoroughly (usually after minimum one hour).
- To monitor the cooler, the temperature limit function can be used (chap. 6.4.5 and chap. 6.4.15).
- The controller function cannot be used together with the pH value determination.
- The pH value is not transmitted to HART and PROFIBUS interfaces.

For the first entry to the parameter setting, you have to insert your specialist code (s. page 21). To enter the menu, proceed as follows:

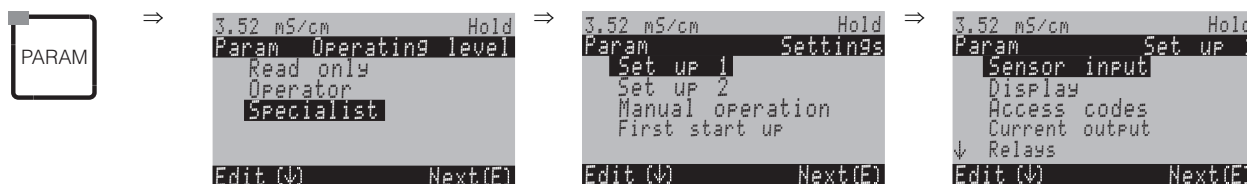



CODE	CHOICE (default = bold)	INFO
A1	One circuit CH1 One circuit CH2 Combined circuits Independent circuits Comb. circuits look-ahead Ind. circuits look-ahead	Select measuring principle (only for two-circuit device) One circuit CH1 / CH2 = measurement via sensor input 1 or 2 Combined circuits = measurement via both sensor inputs with the option of creating a characteristic value (see next field) Independent circuits = independent measurement via both sensor inputs Combined / Independent circuits look-ahead = look-ahead control with combined / independent circuits measurement (only for instruments with 2 current outputs) Note! ■ If a two-circuit device is configured as such, it keeps these settings even if a transmitter (circuit) is removed or is defective. ■ If, with a defective transmitter, the error message E006, E007 is not required, then you can switch the device to "one circuit". As each relay is assigned to a circuit (alarm, rel. 1, rel. 2 to input 1; rel. 3, 4, 5 to input 2), you should keep in mind that, in such a case, functions which access the deactivated relay are no longer functionable.
A2	CH1 – CH2 CH2 – CH1 CH1/CH2 CH2/CH1 (CH1 – CH2)/CH1 (CH2 – CH1)/CH1 (CH1 – CH2)/CH2 (CH2 – CH1)/CH2 pH (CH1 – CH2; VGB)	Select characteristic value (only combined circuits) Here, you can define a process-related characteristic value as a further output parameter. Note! For determination of the pH value see page 31.

CODE	CHOICE (default = bold)	INFO
A3	Mode: Cond. Unit/ auto Medium Comb. unit %	Select operating mode (only combined circuits) If the operating mode changes, the user settings are automatically reset. The settings you make here apply to both measuring circuits. Mode: Cond. (conductivity), resistivity (with conductive sensors), concentration (with inductive sensors) Unit (with Cond. operating mode, difference calculation): auto, $\mu\text{S}/\text{cm}$, mS/cm, S/cm, $\mu\text{S}/\text{m}$, mS/m, S/m Unit (with resistivity operating mode, difference calculation): auto, $\text{k}\Omega\cdot\text{cm}$, $\text{M}\Omega\cdot\text{cm}$, $\text{k}\Omega\cdot\text{m}$. The optimum unit is automatically selected with "auto".  Note! If pH is used as combined unit, Cond. operating mode is preset. Medium (with "concentration" operating mode): NaOH, HNO₃, H₃PO₄, H₂SO₄, Table 1 to 4 Unit with concentration operating mode: %, for customer specific tables. see Chp. 6.4.7 Comb. unit (with ratio calculation): Unit of the characteristic value defined in the previous field Options: none, % or pH value (conductive sensors only)
A4	Measuring circuit 1 Measuring circuit 2	Select measuring circuit
Measuring channel 1 (or 2):		
AA1	Mode: Cond. Unit/medium auto	Select the operating mode (not for combined circuits) If the operating mode changes, the user settings are automatically reset. Mode: Cd. (conductivity), resistivity (with conductive sensors), concentration (with inductive sensors) Unit (with Cond. / resistivity operating mode): auto, $\mu\text{S}/\text{cm}$, mS/cm, S/cm, $\mu\text{S}/\text{m}$, mS/m, S/m / auto, $\text{k}\Omega\cdot\text{cm}$, $\text{M}\Omega\cdot\text{cm}$, $\text{k}\Omega\cdot\text{m}$ The optimum unit is automatically selected with "auto". Medium (with "concentration" operating mode): NaOH, HNO₃, H₃PO₄, H₂SO₄, Table 1 to 4 Unit with concentration operating mode: %, for customer specific tables. see Chp. 6.4.7
AA2	Cell const.: 1.98cm-1 Cable resist. Installation factor 00.00 Ω 1	Select measuring channel 1 or 2 Cell constant: The exact cell constant is provided in the sensor quality certificate. Cable resistance (for conductive): Enter the cable resistance. Installation factor (only inductive): Enter the installation factor here.
AA3	Main value: 01 s Temp.: 01 s (01 ... 30 s)	Set measured value damping The mean value over the set time is displayed.

6.4.2 Set up 1 – Display


To enter the menu, proceed as follows:

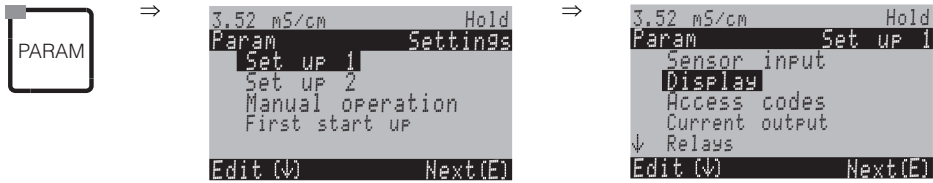

CODE	CHOICE (default = bold)	INFO
B1	E D	Select language Depending on ordered language version. Language versions: Version -A: E / D Version -B: E / F Version -C: E / I Version -D: E / ES Version -E: E / NL Version -F: E / J
B2		Contrast setting as necessary You can increase and reduce the contrast of the display with the +/- keys.
B3	Weekday: Su Day: 01 Month: 04 Year: 01 Time: 08:00	Entry of the date and time Enter the complete date and time here.
B5	°C °F	Select temperature unit °C: Degrees Celsius °F: Degrees Fahrenheit
B6	00000000 (0 ... 9; A ... Z)	Enter your customer specific instrument number 32-digit tag number. This is saved in the DAT module which is obtainable as an option.

6.4.3 Set up 1 – Access codes

To enter the menu, proceed as follows:

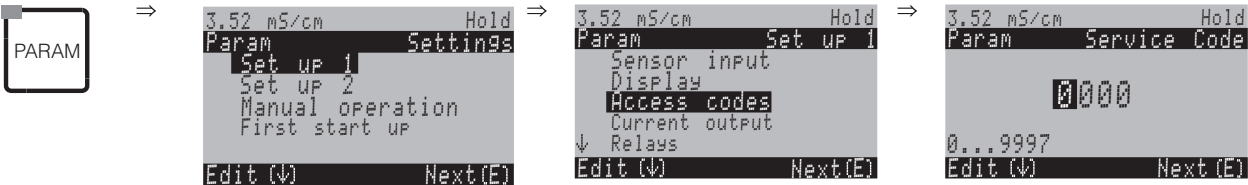

CODE	CHOICE (default = bold)	INFO
D1	0000 (0 ... 9997)	Enter maintenance code In the range 0000 ... 9997, the code can be freely selected. 0000 = no Security Locking.
D2	0000 (0 ... 9997)	Enter specialist code In the range 0000 ... 9997, the code can be freely selected. 0000 = no Security Locking.



Note!
Danger of misuse. Make sure that the codes you enter and the universal code (s. page 21) are protected against misuse by unauthorised persons. Note down the codes and keep them in a place where unauthorised persons do not have access.

6.4.4 Set up 1 – Current outputs

The transmitter is equipped with two current outputs.
To enter the menu, proceed as follows:



⇒

```

3.52 mS/cm      Hold
Param           Settings
  Set up 1
  Set up 2
Manual operation
First start up
Edit (W)      Next (E)
  
```

⇒

```

3.52 mS/cm      Hold
Param           Set up 1
  Sensor input
  Display
  Access codes
  Current output
  Relays
Edit (W)      Next (E)
  
```

CODE	CHOICE (default = bold)	INFO
E1	Current output 1 Current output 2 Create table	Select a current output for which the settings apply.
Current output 1 (or 2):		
EA1	PV input 1 PV input 2 Temperature input 1 Temperature input 2 Combined Continuous controller (only at current output 2)	Select the measured value, which should be output at the current output. Selection possibilities related to the instrument variant and the selected output (see selection table above). PV 1/2 (=primary value): Selection of the primary measured value which you selected, (conduct., conc., resist.) Temperature 1/2: Selection of the temperature to be output to the current output. Combined (only for combined circuits): The characteristic value (e.g. pH value) from Field A3 is output at the current output. Continuous controller (only at current output 2!): The controller actuating variable is output via the current output (see also Controller menu page 56). Note! Danger of data loss. If you change the assignment for the current output from "continuous controller" to a different function after you have configured the controllers, the entire controller configuration (s. page 56) is reset to the default values.
EA2	!!Caution!! The configuration is changed.	Note in display (for changed setting): Cancel by pressing "PARAM" Continue (= confirm change) by pressing "E"
EA3	0 ... 20mA 4 ... 20 mA	Select current range
EA4	!!Caution!! Current output 0...20mA and error current = 2.4 mA leads to uncontrolled behaviour.	Note in display: Error current is in the measuring current range. When the current range is "0 ... 20 mA" and "Min" is selected under Alarm in Field H1, (see page 49). Recommended combinations: Current range 0...20 mA and error current max (22 mA) or Current range 4...20 mA and error current min (2.4 mA)
EA5	Linear Logarithmic Table 1 ... Table 4	Select the characteristic Linear: The characteristic is linear from the lower to the upper value. Logarithmic: The characteristic is logarithmic from the lower to the upper value. Table: You can select four different tables.

CODE		CHOICE (default = bold)	INFO
	Linear:		
	EAA1	0/4 mA: 0.000 $\mu\text{S}/\text{cm}$ / 00.00 % / -35.0 °C / pH = 7.0 20 mA: 02000 mS/cm / 99.99 % / 250.0 °C / pH = 11.0	Entry of the upper and lower measured value limits Entry of the measured values at which the minimum /maximum current value is applied to the outputs.
	EAA6	Linear characteristic active.	Note in display: The linear characteristic is activated after confirmation by pressing "E". Cancel by pressing "PARAM".
	Logarithmic:		
	EAB1	20 mA: 02000 mS/cm / 99.99 % / 100.0 °C / 0500 $\text{M}\Omega\text{-cm}$ / pH = 11.0	Entry of the upper measured value limits Entry of the measured values at which the maximum current value is applied to the outputs. The 0/4 mA value is automatically set to 1 % of the 20 mA value. In fig. 18 you can see the course of the current output signal with logarithmic characteristic. (Distribution: see technical data, p. 104)
	EAB6	Logarithmic characteristic active	Note in display: The logarithmic characteristic is activated after confirming by "E". Cancel by pressing "PARAM".
	Table:		
	EA6	Table active	Note in display: The selected table is active after confirming by "E". Cancel by pressing "PARAM".
	Create table		
	EC1	Table 1 Table 2 Table 3 Table 4	Table selection Select a current output table for editing.  Note! An active table cannot be edited.
	EC2	mS/cm kΩ*cm % ppm mg/l TDS no °C pH (CH1 - CH2; VGB)	Table unit of the measured variable
	EC3	2 ... 10	Enter number of support points (value pairs)
	EC4	mS/cm mA 0000.000 04.00 0010.000 10.00	Enter value pairs (measured value and corresponding current value)  Note! The output characteristic must be strictly monotonously increasing.

CODE		CHOICE (default = bold)	INFO
	EC5	ok Delete pair	Selection: Are the value pairs OK or do you want to delete pairs.
	EC6	Table valid	Note in display: The table is active after confirming by "E". Cancel by pressing "PARAM".

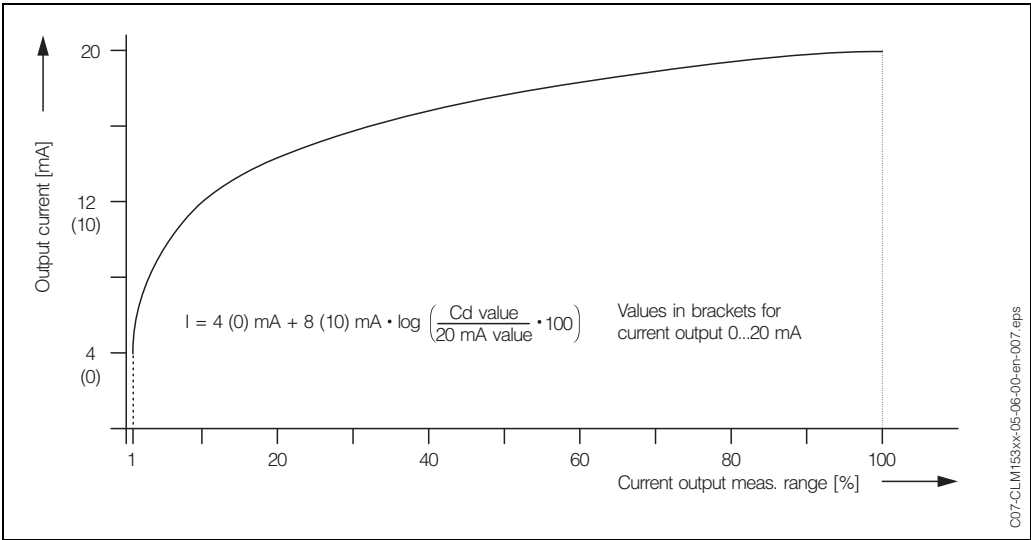


fig. 16: Current output signal with logarithmic characteristic

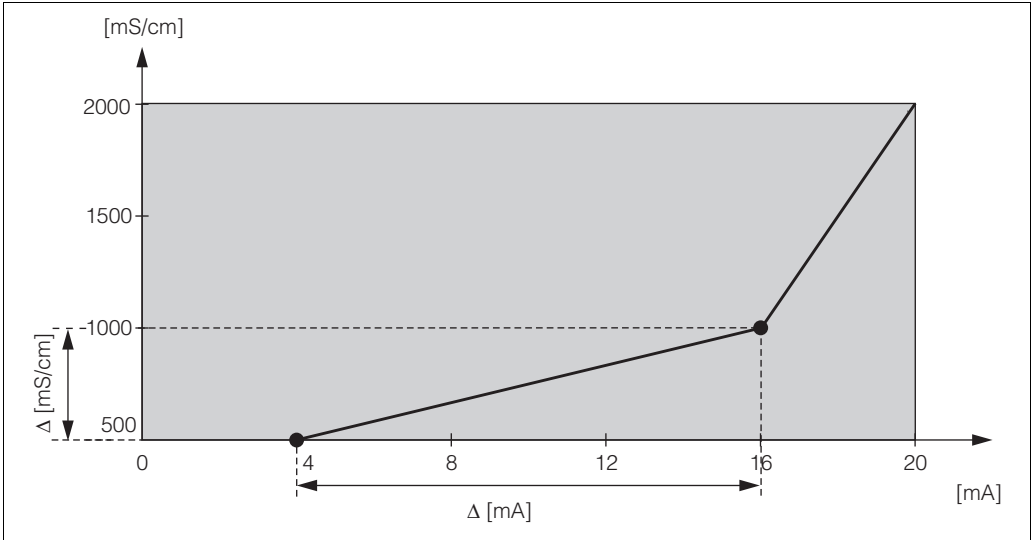


fig. 17: Customer specific current output characteristic



Note!
The controller function "continuous controller" can only be assigned to current output 2.

One-circuit instrument		Two-circuit instrument	
Current output 1 (Terminals 31 +, 32 –)	Current output 2 (Terminals 33 +, 34 –)	Current output 1 (Terminals 31 +, 32 –)	Current output 2 (Terminals 33 +, 34 –)
Conduct./conc./resist. Temperature	Conduct./conc./resist. Temperature Continuous controller	Cond./conc./resist. 1 Cond./conc./resist. 2 Temperature input 1: Temperature input 2	Cond./conc./resist. 1 or 2 Temperature input 1 or 2 Characteristic value Continuous controller

6.4.5 Set up 1 – Relays

To enter the menu, proceed as follows:



CODE	CHOICE (default = bold)	INFO
F1	NAMUR: off Relay 1: no Relay 2: no Relay 3: no Relay 4: no Relay 5: no	Contact functions Depending on the equipment available, you can assign the function of up to 5 relays here. When you switch on the status message acc. to NAMUR NA64, relays 1 and 2 are assigned and are not available for another function, (compare page 15). Selection: No / Controller / Limit 1 / 2 / 3 / 4 / 5 / CCW / CCC Controller: Controller control using relay Limit: Limit switch function (s. chap. 6.4.15) CCW: Chemoclean water. Water supply for the Chemoclean function. CCC: Chemoclean Cleaner. Cleaner supply for the Chemoclean function.(Together, CCC and CCW form the "Chemoclean" function. You can find information on Chemoclean on page 73). The limit value contacts are configured in the menu "PARAM" → "Set up 2" → "Limit switch". The controller contacts are configured in the menu "PARAM" → "Set up 2" → "Controller settings". Note! ■ Danger of data loss. If the controller is already completely configured for output via relay and you reduce the number of relays assigned to the controller, the entire controller configuration (s. page 56) is reset to the default values. ■ If you change the relay assignment for the controllers, you must use the controller menu (s. page 56) to reassign a relay all the functions selected there. Example: Relays 4 and 5 are assigned to the controller and you change the controller assignment to relays 5 and 6 (number of relays remains 2) (no data loss, providing the number of assigned relays is not reduced!). ■ You can only activate NAMUR if the required relays 1 and 2 (compare page 15) are free. ■ If you want to use a limit switch function (s. chap. 6.4.15), first select the limit switch function in the menu "PARAM" → "Set up 1" → "Relays" for a relay and configure this in the menu "PARAM" → "Set up 2" → "Limit switch". Activate the contact with "Function: on".

CODE	CHOICE (default = bold)	INFO
F2	Active open contact Active closed contact	Selection acc. to NAMUR: (only, if NAMUR is activated) Assignment of NAMUR contacts as "active open" contact (= normally closed contact, opens when relay active) or "active closed" contact (= normally open contact, closes when relay active). If the NAMUR function is enabled, the Alarm, Relay 1 and Relay 2 contacts are given the following functions: If the NAMUR function is enabled, the Alarm, Relay 1 and Relay 2 contacts are given the following functions: ■ "Failure" = Fault-signalling contact (terminals 41/42): Failure alarms are active if the measuring system is not working correctly or if process parameters have reached a critical value. ■ "Maintenance required" = Relay 1 (Terminals 47/48): Warning messages become active when the measuring system is working correctly but requires maintenance or a process parameter has reached a value which requires intervention. ■ "Function check" = Relay 2 (Terminals 57/58): This contact is active during calibration, maintenance, configuration and during the automatic cleaning/calibration cycle.
F3	Active open contact Active closed contact	Select controller contacts as active open contact or active closed contact.
F4	Active open contact Active closed contact	Select limit values as active open contact or active closed contact.
F5	Active on Active pulse	Contact type: Fault-signalling contact (only, when NAMUR function = off) Active on = Active for as long as an error is present. Active pulse = Active for 1 second when an alarm signal occurs
F6	Chemoclean is always an active closed contact.	Note in display (only, when the full Chemoclean function is selected in field F1, which means CCC and CCW) With the Chemoclean function, the valves of injector CYR10 are effected with an active closed contact.

6.4.6 Set up 1 – Temperature

Temperature compensation must only be carried out in the Conductivity operating mode (operating mode selection, Field A1, p. 33).



Note!

The settings described in this chapter are not effective for the concentration operating mode. If you use the predefined concentration tables, the temperature will be compensated without further configuration. If you use the customer specific tables, configure the temperature compensation as described in Chp. 6.4.7.

The temperature coefficient α indicates the relative change in conductivity per degree of temperature change. It depends on both the chemical composition of the solution as well as on the temperature itself.

To include the dependency, different types of compensation can be selected in the Mycom S CLM153 :


- Linear compensation
- NaCl compensation
- Compensation via table (four different tables are available)
- NaCl ultrapure water compensation (neutral compensation)
- HCl ultrapure water compensation (acid compensation)

Linear compensation

The conductivity change between two temperatures is taken as constant (i.e. $\alpha = \text{const.}$, see adjacent fig. 18.).

You can edit this α value in linear compensation.

Likewise, you can enter the associated reference temperature. Please refer to the data sheets for the reference temperature.

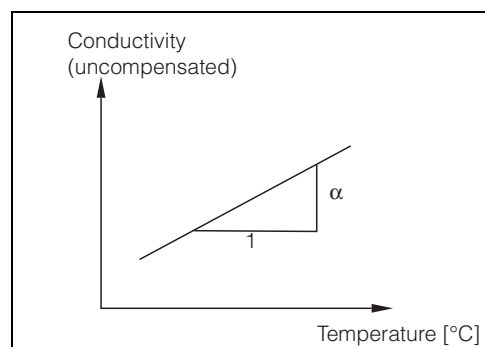


C07-CLM153xx-05-06-00-en-001.eps

fig. 18: Linear temperature compensation

NaCl compensation

For NaCl compensation (in accordance with IEC 60746), a fixed non-linear curve is stored which determines the relationship between the temperature coefficient and the temperature. This curve applies to low concentrations up to 5% NaCl.

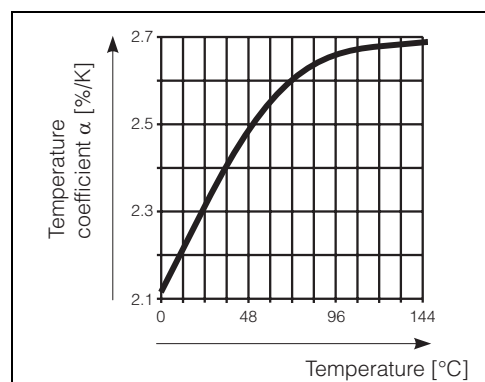

C07-CLM153xx-05-06-00-de-002.eps


fig. 19: NaCl compensation

Temperature compensation with table

The following conductivity data of the medium to be measured are required if using the alpha table function for temperature compensation:

Value pairs of temperature T and conductivity κ with:

- κ for the reference temperature T_0 and
- $\kappa(T)$ for temperatures which occur in the process.

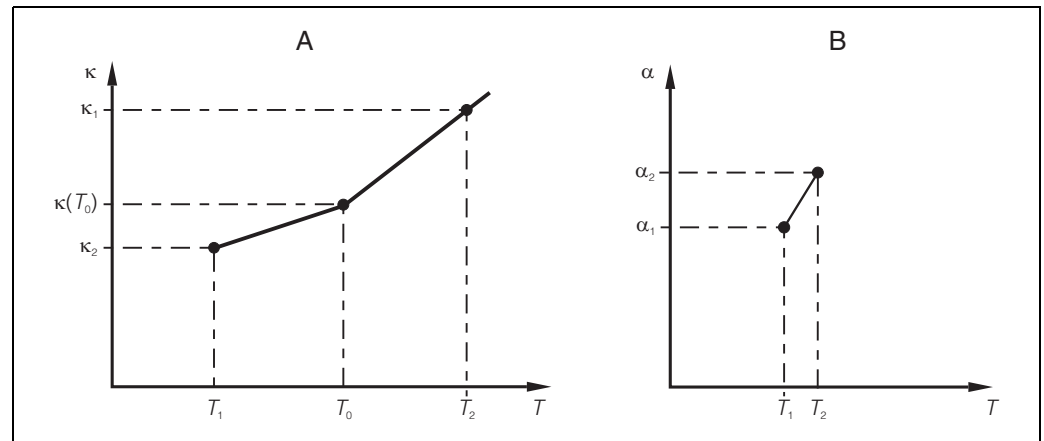

C07-CLM153xx-05-06-00-xx-003.eps

fig. 20: Data required and α values determined with temperature compensation with table

- A Required data
B Calculated α values

Use the following formula to calculate the α values depending on the temperatures occurring in your process:

$$\alpha(T) = \frac{100}{\kappa(T_0)} \cdot \frac{\kappa(T) - \kappa(T_0)}{T - T_0}; (T \neq T_0)$$

Enter the α - T value pairs calculated with this formula into the table in Field GBB3. The transmitter is then ready for operation.

Ultrapure water compensations (for conductive sensors)

For pure and ultrapure water, algorithms are saved in the transmitter that account for the self-dissociation of ultra pure water and its strong temperature dependency. They are used for conductivities of approx. 100 $\mu\text{S}/\text{cm}$ verwendet.

Two compensation types are available:

- NaCl ultrapure water compensation: It is optimised for pH neutral impurities.
- HCl ultrapure water compensation: It is optimised for measurement of the so-called acid conductivity after a cation exchanger. It is also suitable for NH_3 and NaOH .



Note!

- The ultrapure water compensations always refer to a reference temperature of 25 °C / 77 °F.
- The lowest indicated conductivity is the theoretical limit value of ultrapure water at 25 °C/ 77°F, i.e. 0.055 $\mu\text{S}/\text{cm}$.

Temperature configuration menu

To enter the menu, proceed as follows:



CODE	CHOICE (default = bold)	INFO
G1	Temperature Create table Reference temperature	Selection for temperature compensation Temperature = automatic (ATC) or manual (MTC) temperature compensation. Create alpha table: Enter conductivity/temperature value pairs for a temperature compensation by means of the table created. Reference temperature: The temperature to which you apply to.
Temperature:		
GA1	Measuring circuit 1 Measuring circuit 2	Select the measuring circuit you wish to configure.
Measuring circuit 1 (or 2, optional):		
	ATC CH1 ATC CH2 MTC MTC+Temp	Select temperature compensation channel 1/2 ATC: Automatic temperature compensation via temperature sensor MTC: Temperature compensation via manual value entry MTC+Temp: Temperature compensation via manual temperature entry. The displayed temperature, however, is measured by the temperature sensor.
GAA1	Pt 100 Pt 1000 NTC 30k	Select temperature sensor channel 1/2
GAA2	Temp.comp.: linear Alpha value: 2.10%/K Actual temp.: 25.0 °C Offset: 0.0 °C	Temperature compensation channel 1/2 Temp. comp.: Selection of the temperature compensation – none, linear, NaCl, Table 1 to 4, pureNaCl (conductive sensors), pureHCl (conductive sensors) Alpha value: Entry of the conductivity coefficient α (with linear compensation). Actual temp.: The measured temperature is displayed. Offset: Temperature difference between measured and output temperature (–10 ... +10 °C).
Create table:		
GB1	Table 1 Table 2 Table 3 Table 4	Select table Select a table to edit.
GBB2	01 (1 ... 10)	Entry of the number of support points (value pairs) Value pair: Temperature and conductivity coefficient α .

CODE		CHOICE (default = bold)	INFO
	GBB3	°C 000.0 %/K 00.00	Entry of the value pairs Enter temperature and conductivity coefficient, (number of value pairs required = number of support points desired in Field GBB2).
	GBB4	OK Delete element(s)	Selection: Are the value pairs OK or do you want to delete elements?
	GBB5	°C 020.0 °C %/K 025.0 °C 02.00 04.00	Delete: Select the rows to be deleted, delete them with  and confirm this with "E".
	GBB6	Valid table	Note in display: The table is active after confirmation by pressing "E". Cancel by pressing "PARAM".
	Reference temperature:		
	GBC1	For laboratory measurement: 25.0 °C (-35 ... +250 °C)	Entry of the reference temperature to which the medium temperature should be compensated. Here, enter the temperature at which the α value was determined, (you can find this temperature in the data sheets from which you also took the α value).  Note! The ultrapure water compensations always refer to a reference temperature of 25 °C / 77°F.

6.4.7 Set up 1 – Concentration

The transmitter can convert conductivity values to concentration values. To do so, you must first switch the operating mode to concentration measurement (s. page 33, Field A3).

Then select the basic data to which the concentration measurement should refer. These data are already stored in the transmitter for the most common substances. You can select one of these substances in Field A3 / AA1 (Chp. 6.4.1).

You can also determine the concentration of a sample which is not stored in the device. For this, you require the conductivity characteristics of the medium. To get the characteristics, you can either refer to the data sheets of the medium or determine the characteristics your self.

1. To do so, create samples of the medium with the concentrations occurring in the process.
2. Measure the uncompensated conductivity of these samples at temperatures which likewise occur in your process.
 - For variable process temperature:
If the variable process temperature should be taken into account for concentration measurement, you must measure the conductivity of each sample created at two different temperatures at least, (ideally at the lowest and highest process temperature). However, the difference between the temperatures must be at least 0.5 °C. A minimum of four samples is necessary, since the transmitter requires a minimum of four references.
 - For constant process temperature:
Measure the differently concentrated samples at this constant process temperature. Again, a minimum of four samples is necessary for four references.

Impermissible curve profiles

The characteristics received from the measuring points must be extremely monotone increasing or extremely monotone decreasing in the range of the process conditions. Therefore, neither maxima / minima nor ranges with a constant behaviour can occur. Curve profiles such as those in fig. 21 are not permitted.

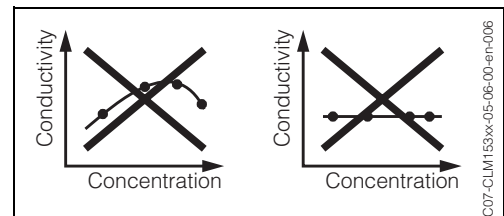


fig. 21: Impermissible curve profiles

Finally you should have measuring data which are similar to those shown in the following figures:

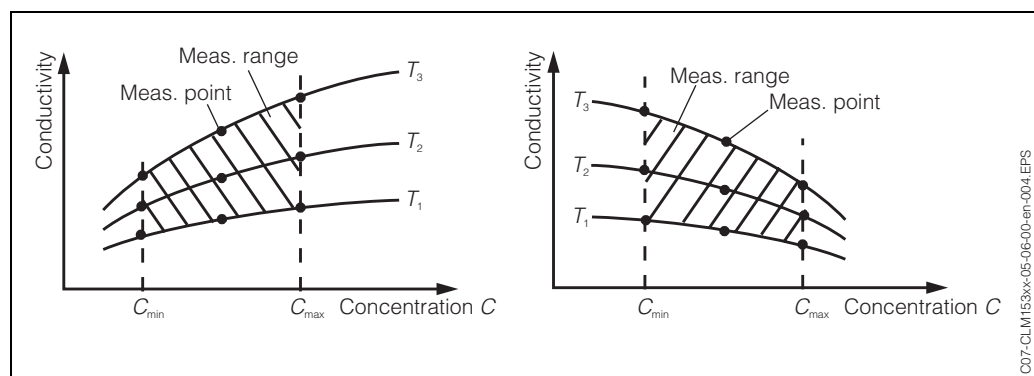


fig. 22: Measuring data in the event of variable process temperature

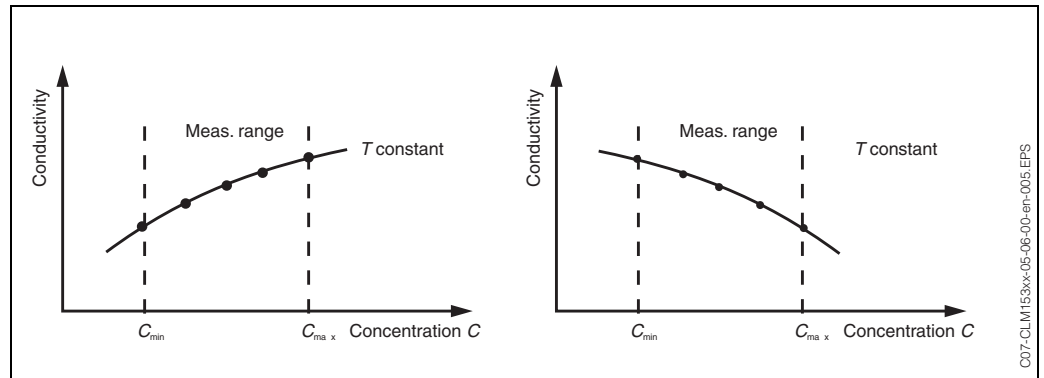


fig. 23: Measuring data in the event of constant process temperature





Note!

- Danger of inaccuracy. Please ensure that the concentrations and temperatures measured for your samples also correspond to the measuring range of the process. If the measured values of the process are outside the range of your sample values, this considerably reduces the level of accuracy and the device generates an error message.
- You can work without error messages from the start of measuring range if you enter an additional triple value set with 0 $\mu\text{S}/\text{cm}$ and 0% for each temperature used, with ascending characteristic (see diagrams above).
- In case of concentration measurement, temperature compensation is performed automatically using the entered table values. Therefore, the compensation set in chap. 6.4.6 is not active.

Enter the three characteristic quantities (triple value set with uncompensated conductivity, temperature and concentration) for each measured sample into the field Z5.

To enter the menu, proceed as follows:

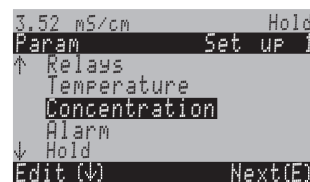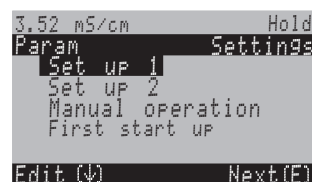

CODE	CHOICE (default = bold)	INFO
Z1	1 (0.5 ... 1.5)	Select the correction factor If it is necessary, you can select a correction factor for the user table here.
Z2	Table 1 Table 2 Table 3 Table 4	Select table Select the table to be read or edited. If you are editing a curve, you should select another curve for calculating the current readings.
Z3	% ppm mg/l TDS ohne	Select concentration unit
Z4	4 (4 ... 20)	Entry of the number of table support points Each support point consists of a set of three numbers (see above).

CODE	CHOICE (default = bold)	INFO
Z5	mS/cm ppm °C 000.00 00.00 000.0 000.00 00.00 000.0 000.00 00.00 000.0 000.00 00.00 000.0 Expl.: mS/cm % °C 223 94.0 50 331 94.0 75 450 94.0 100 212 95.0 50 315 95.0 75 429 95.0 100 157 98.0 50 236 98.0 75 322 98.0 100	Entry of triple pairs Entry of minimum 4 triple pairs for conductivity (uncompensated), concentration (with the unit selected above) and the corresponding temperature.  Note! Enter the values in the order of increasing concentration (see opposite example).
Z6	OK Delete element(s)	Selection: Are the value pairs OK or do you want to delete elements?
Z7	Valid table	Note in display: The table is active after confirmation by pressing "E". Cancel by pressing "PARAM".

6.4.8 **Set up 1 – Alarm**

The transmitter continuously monitors the most important functions. If an error occurs, an error message (list of all error messages s. page 92) is set, which can trigger one of the following actions:

- The fault-signalling contact is made active
- Current output 1 outputs the set error current (2.4 or 22 mA).
 Current output 2 outputs the set error current, if it has not been configured for the "Continuous controller" function.
- Chemoclean cleaning is started



In the list of error messages on page 92 you can see how the error numbers are assigned according to the factory settings. However, in the "ALARM" menu, you have the option of outputting the error messages individually to the alarm relay, the current output or as a cleaning trigger.



Note!

- Please refer to page 92 for the complete list of possible error messages.
- Errors E001 to E029 are assigned to NAMUR functions and cannot be assigned individually.

To enter the menu, proceed as follows:

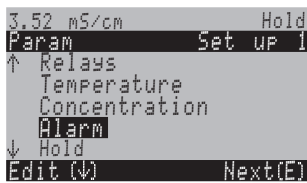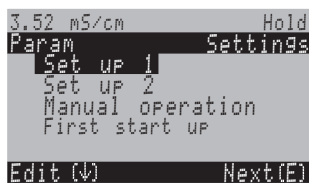

CODE	CHOICE (default = bold)	INFO
H1	Min (2.4 mA) Max (22 mA) off	Selection for error current Set the error current at which an error message is active.
H2	!!Caution!! Current output 0...20mA and error current = 2.4 mA leads to uncontrolled behaviour.	Note in display: Error current is in the measuring current range. If, in Field EA3, the current range is "0 ... 20 mA" and "Min" is selected under Alarm in Field H1. Recommended combinations: Current range 0...20 mA and error current max (22 mA) or Current range 4...20 mA and error current min (2.4 mA)
H3	0000 s (0 ... 2000s)	Entry of alarm delay Delay between error occurrence and alarm trigger.
H4	Function off Service: 100 Failure 200	Alarm for characteristic value monitoring (only combined circuits) Monitoring of measured value difference for two-circuit measurement. Entry of the maximum permitted difference at which the service or failure alarm should be triggered. If the service threshold is exceeded, the error E038 is triggered. If the failure threshold is exceed, the error E019 is triggered.
H5	No. E025 A On I On CC On	Error/contact assignment Each error can be assigned individually: No. = error number E025 (only display) A = Assignment to the alarm relay (activate/ deactivate). An active error triggers an alarm. I = This error triggers an error current CC = Chemoclean®. This error message triggers cleaning.
H6	Function: off Time input: 0000 s (2...9999s)	Dosing time alarm Function: Switch on/off the function "Alarm when dosing time exceeded". Time input: Entry of the maximum allowed dosing time. After this time has elapsed, an error is output.

6.4.9 Set up 1 – Hold

Hold function = "Freezing the outputs"

The current outputs can be "frozen" for each menu. This means that the value which you define in this menu is output. With hold, "Hold" appears in the display.


This function can also be activated externally via the hold input, (see wiring diagram on page page 13, digital input E1). The on-site hold has a higher priority than an external hold.



Note!

- If a hold is active, no programme can be started.
- If current output 2 is configured for the controller, it complies with the controller hold (see Field I5).

To enter the menu, proceed as follows:

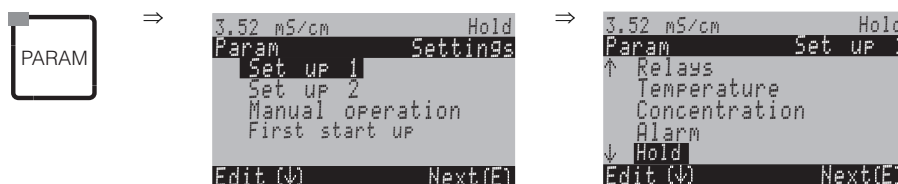

CODE	CHOICE (default = bold)	INFO
I1	CAL DIAG PARAM On On On	Selection: Automatic hold active when: CAL = Calibration DIAG = Service/Diagnosis PARAM = Parameter entry menu
I2	Last Set Min (0/4 mA) Max (22 mA)	Select the current for hold Last = The current value is "frozen" Set = The value set in Field I3 (below) is output for hold. Min / Max = The minimum or maximum current value is output.
I3	000% (0 ... 100%)	Enter Hold current (only for Set) Number settable from 0% = 0/4 mA to 100% = 20 mA
I4	010 s (0 ... 999s)	Enter hold delay time The hold remains active for the given hold delay time after leaving the CAL, PARAM, DIAG menus. During the hold delay time, the "Hold" indicator flashes in the display.
I5	Freeze actuating variable: Yes no	Controller hold Freeze actuating variable (dosing): Yes: During an active hold, the last actuating variable is output. No: During a hold, no dosing takes place. PWM or PFM relays remain in the dropped-out state. An actuator drive is controlled until it is closed. Note! If the set value is output via an actuating variable with feedback, the actuator remains active. It also reacts in the hold should the position suddenly change.

6.4.10 Set up 1 – Parameter sets

Use this item to enter complete parameter sets for a maximum of four media. You can set the following individually for each parameter set:

- Operating mode (conductivity, temperature, ...),
- Temperature compensation,
- Current output (main parameter and temperature),
- Concentration table,
- Limit relay.

Assignment of the binary inputs

You can switch the parameter sets (measuring ranges) externally by means of the binary inputs (MRS). To do so, in Field J1 select the number of inputs which should be controlled externally for measuring range switching:

Field J1: Number of inputs	Function
0	You can activate the four parameter sets by means of the local operation. The parameter set cannot be switched by means of the binary inputs. The binary input 1 can be used for external hold.
1	You can switch between two parameter sets by means of the binary input 2. The binary input 1 can be used for external hold. No measuring range can be activated by means of the local operation.
2	You can switch between four parameter sets by means of the binary inputs 1 and 2. No measuring range can be activated by means of the local operation.

Configuration of the four parameter sets (Example: CIP cleaning)

Field No.	Setting	Parameter set			
		1 (e.g.: beer)	2 (e.g.: water)	3 (e.g.: caustic)	4 (e.g.: acid)
	Operating mode	Conductivity	Conductivity	Concentration	Concentration
	Current output	1 ... 3 mS/cm	0.1 ... 0.8 mS/cm	0.5 ... 5 %	0.5 ... 1.5 %
	Temperature compensation	User tab. 1	Linear	–	–
	Concentration table	–	–	NaOH	User tab.
	Limit values	on: 2.3 mS/cm off: 2.5 mS/cm	on: 0.7 µS/cm off: 0.8 µS/cm	on: 2 % off: 2.1 %	on: 1.3 % off: 1.4 %
Binary input 1		0	0	1	1
Binary input 2		0	1	0	1



Note!

- If the USP function and/or controller is activated, the parameter set cannot be switched since the inputs for parameter set switching (MRS) are no longer available. The menu is then no longer available. The parameter set 1 configured in the remaining "PARAM" menu is then automatically used.
- In measuring mode, the active parameter set is displayed at the right side of the head line.

To enter the menu, proceed as follows:




CODE	CHOICE (default = bold)	INFO
J1	Num. used input: 0 (0 ... 2) Edit PS: 1 (1 ... 2 o. 1 ... 4) Act. PS: 2 (1 ... 2 o. 1 ... 4)	Select the parameter set (measuring range) Num. used input: Number of inputs by means of which parameter sets can be switched externally (0...2). Edit PS: Selection of the parameter set to be edited. The parameter sets are always configured by means of the local operation or the PC Tool (1...2, if num. used input = 1; otherwise 1...4). Act. PS: Activation of a parameter set (for num. used input=0 only; if num. used input=1 or 2, the parameter set is selected via the binary inputs).
J4	Channel 1 Channel 2 Sensor input Current out Limit switch Delta alarm	Selection for configuration Channel 2: two-circuit instruments only Sensor input: combined circuits only Delta alarm: combined circuits only
Channel 1 (or 2):		
JA1 / JB1	Cond. Resist. Conc.	Select operating mode not for combined circuits
JA2 / JB2	Temp.comp.: linear TC value: 2.10 %/K	Temperature compensation (conductivity and resistivity only) Temp.comp.: Temperature compensation selection – no TC, linear, NaCl, Table 1 to 4, pureNaCl, pureHCl TC value: Enter temperature coefficient (with linear compensation only).
JA3 / JB3	NaOH HNO3 H2SO4 H3PO4 Table 1 Table 4	Medium (concentration only)
Sensor input		
JC1	Cond. Resist. Conc.	Select operating mode combined circuits only; common operating mode; if pH is used as combined unit, operating mode is preset to Cond.
Current out		
JD1	Current out 1 Current out 2	Select the current output which shall be configured

CODE		CHOICE (default = bold)	INFO
	Current out 1 (or 2)		
	JDA1/JDB1	PV CH1 PV CH2 Temp. CH1 Temp. CH2 combined	Select measured value
	JDA3/JDB3	Function: linear 0/4 mA: 0.000 µS/cm 20 mA: 200 mS/cm	Output configuration Function: linear, logarithmic, table 1 ... 4
	Limit switch		
	JE1	Limit switch 1 Limit switch 2 Limit switch 3 Limit switch 4 Limit switch 5	Select the limit switch that you want to configure.
	Limit switch 1 / 2 / 3 / 4 / 5		
	JEA1/JEB1/ JEC1/JED1 /JEE1	Function: off On value: 2000 mS/cm Off value: 2000 mS/cm On delay: 0 s Off delay: 0 s Alarm limit: 2000 mS/cm	Configuration of limit switches Detailed information see chap. 6.4.15.  Note! Assignment of limit switches to the measured variable is done in the "Setup 2 → Limit switch" menu. It is independent from the parameter sets (s. chap. 6.4.15).
	Delta alarm		
	JF1	Function: off Service: 10.50 pH Failure: 11.00 pH	Alarm for the characteristic value for combined circuits If the service threshold is exceeded, the error E038 is triggered. If the failure threshold is exceed, the error E019 is triggered.

6.4.11 Set up 1 – Emergency switching

If the hardware (e.g. sensor or transmitter) is defective, you can change the function of the transmitter using the emergency switching. You can set the sensor of one circuit to the transmitter of the other circuit.

To enter the menu, proceed as follows:

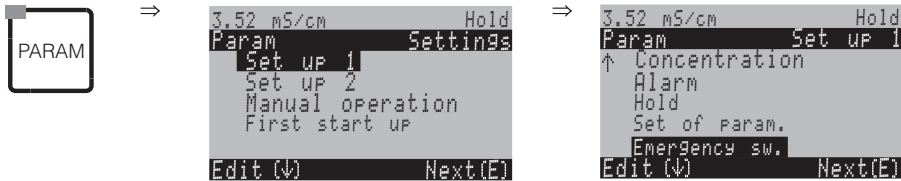


CODE	CHOICE (default = bold)	INFO
N1	Caution! Being switched to one-circuit measurement.	Note in display
N2	Switching off Sensor 1 → input 2 Sensor 2 → input 1	Emergency switching Sensor 1 is set to input 2 or vice versa. The settings you made for the circuits are kept. The circuit data apply after switching, with the exception of the sensor-specific data.


6.4.12 Set up 2 – Data log

The data log records two freely selectable parameters with their date and time. You can start it using the measuring menus:

Use the arrow keys to scroll through the measuring menus until you reach the Record mode of the data logger. Pressing the "Enter" key brings you to the Scroll mode of the data logger. Here you can open the saved measured values with their date and time.


To enter the menu, proceed as follows:

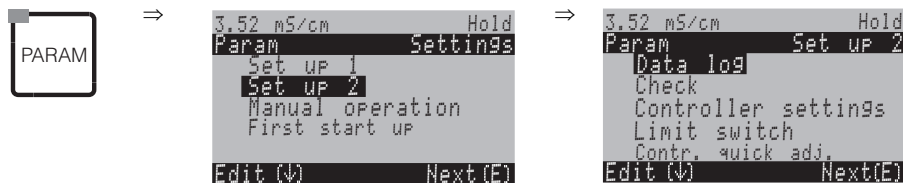

CODE	CHOICE (default = bold)	INFO
K1	Sample time Data log 1 Data log 2 Display log. 1 Display log. 2	Data log settings Using the data log you can record ■ one parameter with 500 sequential measuring points or ■ two parameters each with 500 sequential measuring points. Display log 1/2: You can view the data recorded in the data log.
Sample time:		
KA1	00005s (2 ... 36000s)	Enter sample time Enter the time interval after which the next measured value is recorded in the data log.
Data log 1 (or 2):		
KB1 / KC1	Input: PV CH1 Function: Off	Selection Set the measured value for recording (PV CH1, PV CH2, temp. CH1, temp. CH2, combined) and then activate by means of the "on" function.
KB2 / KC2	Min: 0.00 Max: 2000.00	Set recording range Values outside the defined range are not recorded.
Display log. 1 (or 2):		
KD1 / KE1		View of the recorded data You can call up data recorded in the past with date and time of their recording.

6.4.13 Set up 2 – Check

To enter the menu, proceed as follows:

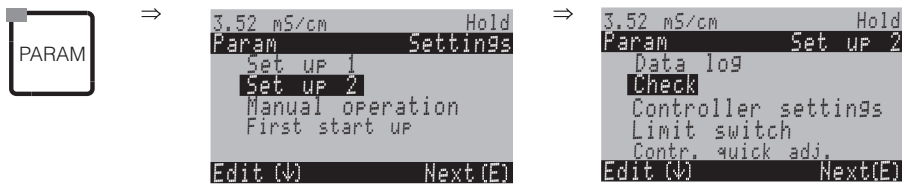

CODE	CHOICE (default = bold)	INFO
L1	PCS input 1: off PCS input 2: off	PCS (= Process check system) time If the measuring signal does not change over the period entered, an alarm is signalled with error message E152. Settable times: off, 1h, 2h, 4h. Monitoring limit: 0.3 % of mean value over the set period of time. Note! An active PCS alarm signal will be deleted automatically as soon as the sensor signal changes.

6.4.14 Set up 2 – Controller settings

Requirements for controller configuration:

You have carried out the following settings **which are necessary for the controller settings** either in the First start up, page 24 or on the appropriate menu page.

If you have not yet made the settings, please do this **before** configuring the controller.

- Specify the relays available for the controllers (Field T17, page 29, or Field F1, page 40).
- Define current output **2** as a continuous controller if you want to control the actuator via a 20 mA interface (Field T19, page 29, or Field EA1, page 36).



Note!

- Danger of data loss. If you assign the relays which are used by the controller with another function (Field F1, page 40), the **entire** controller configuration is reset to the default values.
- If you change the relay assignment for the controllers in the Contacts menu (Field F1, page 40), you must use the Controller menu to reassign a relay to all the functions selected there.
Example: Relays 4 and 5 are assigned to the controller and you change the controller assignment to relays 2 and 3 (number of relays remains 2) (no data loss, provided the number of assigned relays is not reduced!)
- Relays 3, 4 and 5 are located on the additional plug-in card. If you have used one of these relays for the controller function and want/have to remove this card from the device, then we would recommend that you change the controller settings before removing the second card, so that all the relays used by the controller are located on card 1. Otherwise, you cannot use the controller function during the time in which the additional card is not plugged into the device, as the controller needs to access the relays on the second card.
- The controller function is not available with pH value determination by differential conductivity.

Definition of terms


Actuators:	Valves, gate valves, pumps and similar
Upward/ downward controller:	The terms "up" (=upward controller) and "down" (=downward controller) used in the menu are used in relation to the direction of action: Down = The control doses only if the measured value is greater than the setpoint. Up = The control doses only if the measured value is smaller than the setpoint.
Process:	The controller or the process (to simplify matters this will, from henceforth, be referred to as the "process") can be differentiated on account of their different features:
Direction of action, one or two-sided:	One-sided control only works in one of two directions. It influences the process in such a way that the measured value either rises (upward controller) or drops (downward controller). With a two-sided process, control can generally work in both directions, ("up" and "down"). This means that you can both increase and decrease the value of the controlled variable (here = measured value).
Batch or inline process arrangement:	With active control, the batch and inline processes are different in their relationship to the medium current: Pure batch process: The batch container is filled with the medium. During the subsequent batch process, no additional medium is fed in. The change in the measured value is caused only by the control. To be able to compensate for possible so-called "overshoots", use a two-sided control (see above). For as long as the actual value is within the neutral zone, no additional dosing agent is added. Pure inline process: Here, the control works with the medium flowing past. The measured value of the medium in the inflow may be subject to strong deviations for which the control should compensate. The volume of medium which has already flowed past can no longer be influenced by the controller. For as long as the actual value corresponds to the setpoint, the actuating variable has a constant value. The Mycom S controller takes this differing behaviour into account. It is the internal handling of the integral part of the PI or PID controller which is different for these settings. In practice, the most common option is the semi-batch process. Depending on the ratio of inflow to tank size, this process shows the behaviour of an inline or a batch process.
Look-ahead control	To be able to optimally resolve the general problems of a purely inline process, the CLM153 is able to "look into the future" using a second sensor and a flowmeter. This means that the controller can react to strong variations in the inflow at an early stage.
Controlling the actuators	The CLM153 has four different methods for controlling the actuators (see above.) 1. PWM (Pulse-width modulation, "pulse-length controller") Pulse-width modulated outputs aid control e.g. of solenoid valves. With PWM, the internal, continuous actuating variable is output to a relay as a rhythmic signal. The larger the calculated actuating variable, the longer the appropriate contact remains picked up (i.e. the longer the switch-on period t_{ON}; s. fig. 24 is). You can set the period length freely between 1 and 999.9 seconds. The minimum switch-on period is 0.4 seconds. A two-sided process requires two PWM relays or one PWM and a three-point step controller (see below.) One PWM relay on its own can only output one actuating variable. To avoid pulses which are too short, enter a minimum switch-on period. Pulses which are too short are not given to the relay/or the actuators. This benefits the actuator.

2. PFM (pulse-frequency modulation; "pulse-frequency controller")

Pulse-frequency modulated outputs aid control e.g. of solenoid dosing pumps. As with PWM, PFM is output as a rhythmic signal by the relay.

The greater the calculated actuating variable, the higher the frequency of the related contact. The maximum settable frequency $1/T$ is 120 min^{-1} . The switch-on period t_{ON} is constant at approx. 250 mS (s. fig. 24).

Here too, two PFM relays are required for a two-sided process.

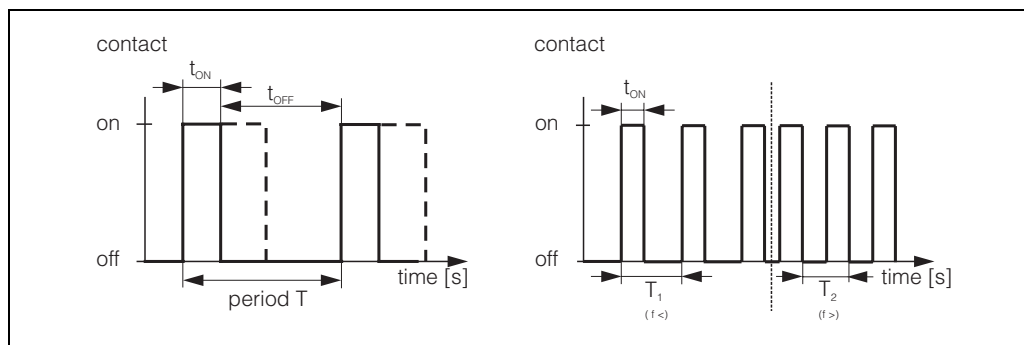

C07-CPM153xxx-05-06-00-en-004.eps

fig. 24: Left: pulse-width modulation (PWM)
Right: pulse-frequency modulation (PFM)

3. Three-point step controller

With Mycom S, this type of control is only possible for one process side ("Up" or "Down"). With two-sided processes, either PWM or PFM must be used for the other process side.

The three-point step controller can only be selected if an analogue input for the actuator feedback is available.

Select this type of control for actuator drives (e.g. valves, butterfly valves etc.), which must be controlled by means of two relays and which have position feedback. Only actuator drives with position feedback are supported. If the "+relay" picks up, the valve opens (flow increases) until the "+relay" drops out again. The "-relay" closes the valve in a similar way.

The Mycom S has an internal position controller which compares the set and actual positions of the valve, (set position from the primary controller and actual position from the position feedback). The relay in question picks up as soon as the position error exceeds the set switching differential X_{SD} . The actuator drive is controlled more frequently and more precisely, the smaller the X_{SD} selected. This also results in a more accurate overall control. However, if the switching differential is too small, there is the risk that the position control starts to oscillate.

For your process, you must find the optimum value between a large switching differential which protects the actuators and a small switching differential which ensures better control quality.

The set motor run time aids valve monitoring.



Note!

If using a driven valve, gate valve or similar, you must determine this motor run time before starting with the menu settings.

4. Analogue (via current output 2, 20 mA)

The current output can be used to output the analogue actuating variable for one or two-sided processes and cannot be combined with the method described above.

- With one-sided processes, the actuating variable range 0% ... 100% (or -100% ... 0%) is represented on the selected current range (0 ... 20 mA or 4 ... 20 mA). The output current is proportional to the actuating variable.
- With a two-sided process, the complete actuating variable range from -100% ... +100% is represented on the given current range. An actuating variable of 0% leads to a current of 10 mA (at 0 ... 20 mA) or 12 mA (at 4 ... 20 mA), (see fig. 25).



Note!
With a two-sided process, it should be noted that the actuator uses this method (also known as "split range").

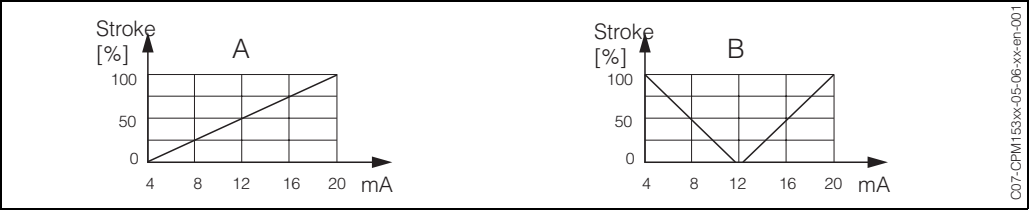


fig. 25: A: Stroke diagram for a control valve
 B: Stroke diagram for two contrarotating control valves ("split range")

You can refer to the following selection aids to find the required hardware equipment level for your process.
This selection is not complete. If you wish to use additional functions such as NAMUR or Chemo-clean, please check to see if you require additional relays (NAMUR: Alarm relay + 2 relays; Chemo-clean: 2 relays).

Selection aid for online processes						
Process Path		Dosing actuators	Required hardware equipment for control			
			Circuits	Relay	Current inputs	Current outputs
1-sided control	looking-ahead · 2-circuit · flow	1 PWM	2	1	1	—
		1 PFM	2	1	1	—
		1 3-point step	2	2	2	—
		1 PWM/PFM	2	2	1	—
		analogue	2	—	1	1
	not looking-ahead	1 PWM	1	1	—	—
		1 PFM	1	1	—	—
		1 3-point step	1	2	1	—
		1 PWM/PFM	1	2	—	—
		analogue	1	—	—	1

Selection aid for online processes

Process	Path	Dosing actuators	Required hardware equipment for control			
			Circuits	Relays	Current inputs	Current outputs
2-sided control	looking-ahead · 2-circuit · flow	2 PWM	2	2	1	–
		2 PFM	2	2	1	–
		1 3-point step	2	3	2	–
		1 PWM/PFM	2	3	1	–
		current output split range	2	–	1	1
	not looking-ahead	2 PWM	1	2	–	–
		2 PFM	1	2	–	–
		1 3-point step	1	3	1	–
		1 PWM/PFM	1	3	–	–
		current output	1	–	–	1

Selection aid for batch processes or slow online processes

Process	Dosing actuators	Required hardware equipment for control			
		Circuits	Relays	Current inputs	Current outputs
1-sided control	1 PWM	1	1	–	–
	1 PFM	1	1	–	–
	1 3-point step	1	2	1	–
	1 PWM/PFM	1	2	–	–
	current output	1	–	–	1
2-sided control	2 PWM	1	2	–	–
	2 PFM	1	2	–	–
	1 3-point step	1	–	1	1
	1 PWM/PFM	1	3	–	–
	current output split range	1	3	–	–

PWM = pulse length proportional

PFM = pulse frequency proportional

3-point step = Three-point step controller

The controller in the CLM153:

The CLM153 contains a multi-faceted PID controller which can be adapted to the process. It has the following features:

- Separate configuration of both process sides,
- Simple adaptation to batch or inline processes,
- Switching option between constant and range-dependent modulation gain.

Relating to the effect on the gain factor, a difference is made between two standard implementations:

- The factor $K_R(X)$ is the total gain (see fig. 26. This is implemented in the CLM153).
- The gain factor $K_P(X)$ is the purely proportional gain.

The following diagram shows the schematic structure of the CLM153 controller. Because of the simplicity of the diagram, the Laplace transform of subfunctions is given.

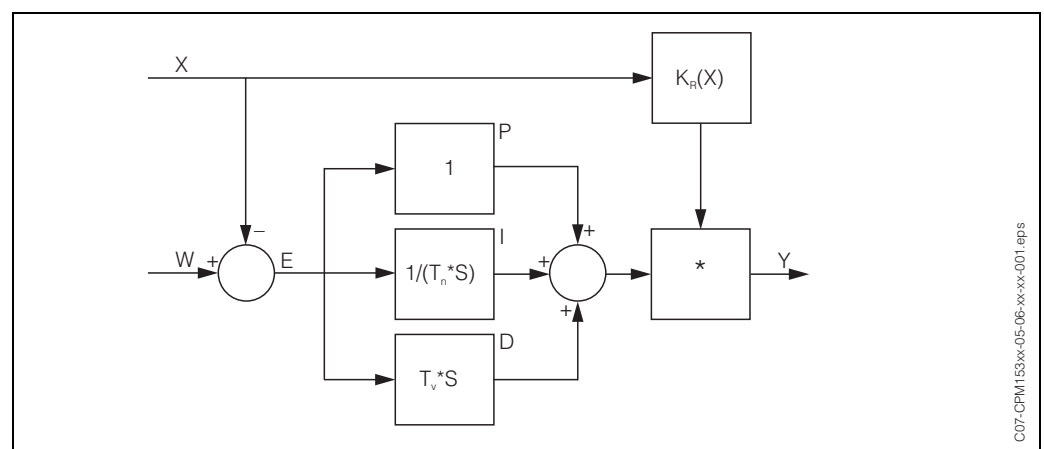


fig. 26: Schematic diagram of the CLM153 controller with $K_R(X)$ as the total gain

X	Actual value
W	Setpoint
E	Control difference
Y	Actuating variable
K_R	Modulation gain (total gain)
T_n	Integral action time (I component)
T_v	Derivative action time (D component)

Range-dependent modulation gain

In contrast to normal PID controllers, with Mycom S you have the option of setting a range-dependent modulation gain in addition to a constant controller gain. With range-dependent gain, the controller gain used depends on the “range”, i.e. on the present actual value.

Areas of application for range-dependent gain are:

- Compensation of non-linearities:
The conductivity process is no longer linear at medium and high concentrations (approx. > 15 %).
- For critical control systems,
you need a control which works very carefully near the setpoint and doses very powerfully in the event of large control difference. If constant controller gain cannot do this to your satisfaction, then you can achieve this by using range-dependent modulation gain.

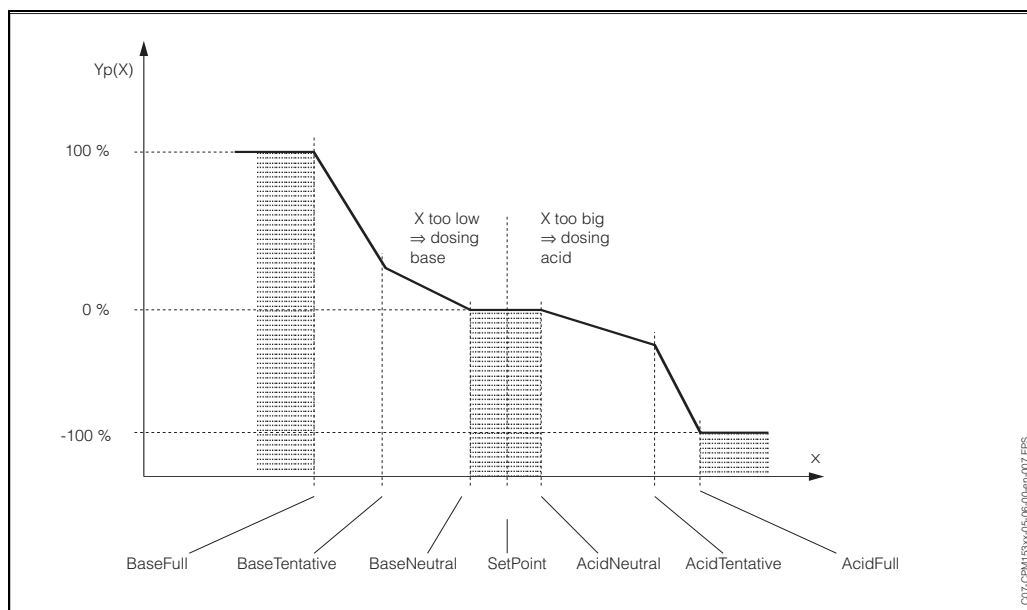


fig. 27: Diagram to describe the most important corner points for control

With such a range-dependent characteristic, a set actuating variable is prescribed to the controller for each measured value.

Neutral zone:

If the actual value (X) is within the neutral zone, then

- the dosing does not take place for the Batch process type,
- also not for the Inline process type and without an I component ($T_n=0$).
- If the controller is configured as a PI or PID controller for the Inline type, the controller decides itself if dosing will be carried out or not. This is dependent on the measured value history.

Points of the characteristic:

For constant control gain ("linear characteristic"), you require:

- Setpoint W,
- Neutral zone
 - Two-sided: "Start of the neutral zone" and "End of neutral zone"
 - One-sided: only one of the two points

For range-dependent modulation gain ("segmented characteristic"), you require two-sided control of all the points.

A point usually consists of two coordinates: an x coordinate (here = measured value) and a y coordinate (here = actuating variable). You only need enter the y coordinates for the optimisation points. For the other points, the CLM153 sets the y coordinates itself.

However, you cannot change the sequence of these defined points. It is, for example, not possible to enter a larger measured value for the "Start neutral zone" than for the setpoint.


Configuring the CLM153

Please configure the relays in the following order:

1. Actuators
2. Sensor technology
3. Feedback (e.g. look-ahead control, position feedback with three-point step controller, if available)
4. Characteristic:

In the user settings (see below) you switch directly to a controller simulation and can check the settings made and change them if necessary.

To enter the menu, proceed as follows:

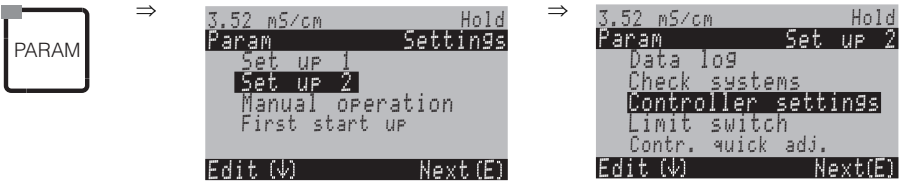


CODE	CHOICE (default = bold)	INFO
M1	off On	Select controller functions 📌 Note! You must activate the controller function after you have configured the controllers in this menu branch.
M2	Batch 1-s. up Batch 1-s. down Batch 2-sided Inline 1-s. up Inline 1-s. down Inline 2-sided	Select the process type, which describes your process. 1-s. = one-sided: The control is either "up" or "down". Two-sided: The control is "up" and "down". You can only select this function if you have defined two controllers (in the "Contacts" menu and/or via the current output).

CODE	CHOICE (default = bold)	INFO
M3	Type Sensor input Feedback Characteristic	Select external hardware For correct operation, you must completely configure these four submenus. Type: here, you can select and configure the methods which the controller uses to output the actuating variable. Sensor input: Here you configure the look-ahead control or switch channels (only with two circuit). Feedback: Here you configure the position feedback of an actuator drive (only with the selection of three PS and position feedback = on; see Fields 162, 165 / 170, 165) Characteristic: Here, you enter the controller parameters (neutral zone, setpoint, etc.). With this selection, you can also reach the controller simulation (see Field ME6).
Type: With selection "one-sided" in Field M2:		
MA1	Up Down	Dosing Select the control type with which you wish to dose.
MA2	Pulse length Pulse frequency 3-point step controller Current output	Select control type
MA3	+relay n.c. -Relay n.c. Motor on time 060.0 s Xsd 4.0 %	Relay selection (for three-point step controller) +Relay: Open the valve further (= increase dosing) -Relay: Close the valve further (= reduce dosing) Selection: n.c. (= not connected). After this, those relays which are released in the Contacts menu are always offered as the default.  Note! If you cannot select a relay here, use the "Contacts" menu to make relays available for the controller function. Motor on time: The time the motor drive requires to move the valve from completely closed to completely open. The CLM153 requires this to be able to calculate the required pick-up time of the relay for any required position change. Xsd: Xsd is the dead zone of the actuator control. A deviation of the actuator position from the calculated set value is not corrected up to the % value that you set here.  Note! The CLM153 expects feedback from the actuator drive about the current valve position via a current or resistance input.
MA4	Relay: n.c. max. pulse fre- 120/min. quency	Relay selection (for pulse frequency) Relay: Relay selection Max. pulse frequency: Input of the maximum pulse frequency. (Pulses with a higher frequency are not forwarded to the relay). (Maximum setting: 120 1/min)
MA5	Relay: n.c. Period: 000.0s t _E min: 000.0s	Relay selection (for pulse length) Relay: Relay selection Period: Period length T in seconds (Range 0.5 ... 999.9 s) t_E min: Minimum switch-on period. (Shorter pulses are not forwarded to the relay and treat therefore the actuators with care).

CODE		CHOICE (default = bold)	INFO
	MA6	0 ... 20mA 4 ... 20 mA	Current output Selection of the current range, which should be output at the current output.
	MA7	0/4 mA 20 mA	Current output Assign the current value which corresponds to 100 % dosing medium provision.
Type With selection "two-sided" in Field M2:			
	MB1	Dosing via: 1 output 2 outputs	Control: (This is only if you selected the constant controller under current output 2.) 1 output: for control using the current output in the "split range" method. Control logics are required which can control two valves/pumps over one current input. 2 outputs: If the valves are controlled with two relays.
	1 Output:		
	MBA1	0 ... 20mA 4 ... 20 mA	Current output Selection of the current range, which should be output at current output 2. The neutral position (= current value which the controller outputs when it is not dosing) is in the middle of the selected range. For 0 ... 20 mA, the neutral position is at 10 mA, for 4 ... 20 mA at 12 mA.
	MBA2	0 (or 4) mA 20 mA	Current output 2 Assign the current value, corresponding to 100 % dosing.  Note! From the current value selection for the dosing of 100 % dosing agent, you can derive the current ranges for up and down dosing, (see fig. 28) in the "split range" method.
			Stroke [%] 100 50 0 4 8 12 16 20 mA down up
	fig. 28: Two-sided control over one current output		
	2 outputs:		
	MBB1	Up: pulse length Down: pulse length	Select the control type Dosing can be carried by carried out using: Pulse length signal Pulse frequency signal Three-point step controller
	MBB2	+relay n.c. -Relay n.c. Motor on time 060.0 s Xsd 04.0 %	Downward dosing: Relay selection (for three-point step controller) Description see above.

CODE		CHOICE (default = bold)	INFO
	MBB3	Relay: n.c. max. pulse fre- quency 1/min.	Downward dosing: Relay selection (for pulse frequency) Description see above.
	MBB4	Relay: n.c. Period: 000.0s t_E min: 000.0s	Downward dosing: Relay selection (for pulse length) Description see above.
	MBB5	+relay n.c. -Relay n.c. Motor on time 060.0 s Xsd 04.0 %	Upward dosing: Relay selection (for three-point step controller) Description see above.
	MBB6	Relay: n.c. max. pulse fre- quency 1/min.	Upward dosing: Relay selection (for pulse frequency) Description see above.
	MBB7	Relay: n.c. Period: 000.0s t_E min: 000.0s	Upward dosing: Relay selection (for pulse length) Description see above.
Sensor input:			
	MC1	Look-ahead control: PV 1 = controller PV 2 = look-ahead	Note in display: Look-ahead measurement (only look-ahead) In First start up, one process with look-ahead control was selected. 📎 Note! Control with look-ahead measurement is only possible in conjunction with a flowmeter and a two-circuit transmitter.
	MC2	Control with: PV 1 PV 2	Electrical assignment: (only redundancy) Selection of with which measured value, control is effective.
	MC3	L_B : 0.5 m L_S : 0.5 m L_E : 1.5 m	System arrangement Enter sensor/dosing point distances: L_S: Distance between the controlling sensor and the down dosing point L_B: Distance between the controlling sensor and the up dosing point L_E: Distance between the controlling sensor and the look-ahead sensor Notes on fig. 29: Sensor 1 is the controlling sensor, sensor 2 is the look-ahead el.

Two-sided pipe flow neutralisation (inline) with forward-locking conductivity measurement

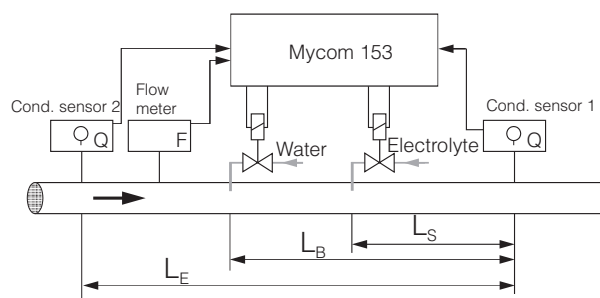

C07-CLM153cx-16-06-00-en-009.eps

fig. 29: Schematic diagram of a two-sided control with look-ahead control

CODE	CHOICE (default = bold)	INFO
MC4	Unit: m ³ /h Unit: s 4 mA value: — 20 mA value: —	Flowmeter volume flow Unit: Entry of the volume flow in m ³ /h or yd ³ /h 4 mA value: Enter minimum flow velocity value. 20 mA value: Enter maximum flow velocity value.
MC5	Diameter 00 mm	Pipe diameter Entry of the internal diameter of the pipe located between the two sensors.
MC6	Function On Limit value 050.0 K _{ffc} =1: 050.0 K _{max} : 1.7 K _{stop} : 1.0	Feedforward control (only if 2 current inputs are available) Feedforward control has a multiplying effect, i.e. the controller actuating variable is multiplied by the gain K _{ffc} (s. fig. 30). Limit value: If the current input signal undershoots the value set here, dosing is stopped (actuating variable = 0). The dosing stop is not active if you enter 0 (= no limit value) here. (Range 0...100%) K_{ffc}=1: Here, enter the current input value in % at which the feedforward gain should have the value 1. At this point the output actuating variable is the same for switched-on or switched-off feedforward control. (Range 0...100%) K_{max}: Here, the value of K _{ffc} is displayed for a current input signal of 100%. K_{stop}: Here, the value of K _{ffc} is displayed for current input signal which is equal to the limit value.

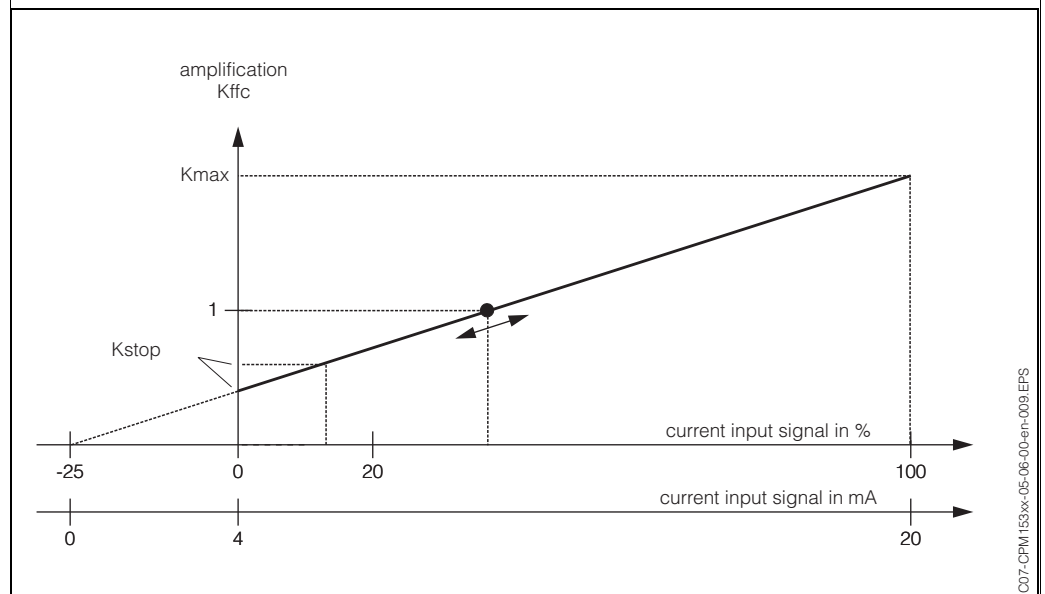


fig. 30: Multiplying feedforward control

Feedback:		
The following selection is dependent on whether you have a resistance or a current input.		
With resistance input		
MD1	0 ... 1 k Ω 0 ... 10 k Ω	Select range for resistance.

CODE	CHOICE (default = bold)	INFO
MD2	act. resistance ____ k Ω	Assign a value for y = 0 % Drive the valve to y = 0 %. The current resistance is displayed. You can change the valve position either manually or by pressing the arrow keys on the transmitter. Confirm the position for y = 0 % by pressing the "E" key.  Note! If you cannot change it using the arrow keys, please check the "Actuators" menu (Field 165) to see if the relays have been assigned to valve control.
MD3	act. resistance ____ k Ω	Assign a value for y = 100 % Drive the valve to y = 100 %. Proceeding as in the previous field.
For current input 1:		
MD4	y = 0 ... 100 % mA: 4 ... 20 20 ... 4	Select current range and assign the percentage range.
MD5	act. mA value: ____ mA	Assign a value for y = 0 % Drive the valve to y = 0 %. The current current value is displayed. You can change the valve position either manually or by pressing the arrow keys on the transmitter. Confirm the position for y = 0 % by pressing the "E" key.  Note! If you cannot change it using the arrow keys, please check the "Actuators" menu (Field 165) to see if the relays have been assigned to valve control.
MD6	act. mA value: ____ mA	Assign a value for y = 100 % Drive the valve to y = 100 %. Proceeding as in the previous field.
Characteristic:		
ME1	Linear characteristic Segmented characteristic	Characteristic type selection Linear characteristic : Corresponds to a constant control gain. Segmented characteristic : Corresponds to a range-dependent control gain.
ME2	Setpoint 1000 mS/cm Start neut 800 mS/cm End neut 1500 mS/cm K _R 1 200 mS/cm K _R 2 200 mS/cm	Characteristic values for linear characteristic (constant control gain) ; K_R Setpoint: The value which should be set. Start neut: Start neutral zone End neut: End neutral zone K_R 1 (only with up dosing): Modulation gain for up dosing K_R 2 (only with down dosing): Modulation gain for down dosing
ME3	Setpoint 1000 mS/cm Start neut. 990 mS/cm End neut. 1010 mS/cm O.pnt. X1 900 mS/cm O.pnt.Y1 0.20 O.pnt. X2 1100 mS/cm O.pnt.Y2 -0.20 Control po. 1 800 mS/cm Control po. 2 1200mS/cm	Characteristic values for segmented characteristic (range-dependent control gain) Setpoint: The value which should be set. Start neut: Start neutral zone End neut: End neutral zone Optimisation point 1 and 2: Entry with x and y coordinates Control point 1: The dosing is 100% up for measuring values < control point 1. Control point 2: The dosing is 100% down for measuring values > control point 2.

CODE	CHOICE (default = bold)	INFO
ME4	Fast process Standard process Slow process User settings	Select process character If you have no experience in setting control parameters, the defaults fast / standard / slow process are intended as an aid to adapting the controller behaviour to the process. Select a default and use the "controller simulation" (see below) to check if these settings are relevant for your process. Enter all the characteristic values yourself with the user settings.
ME5	K_R 1 = K_R 2 = Tn 1 = Tn 2 = Tv 1 = Tv 2 =	Characteristic values for user settings: (K_R 1 and K_R 2 only with linear characteristic; Index 1 only for up dosing, Index 2 only for down dosing) K_R 1: Modulation gain for up dosing K_R 2: Modulation gain for down dosing Tn: integral action time (0.0 ... 999.9 min) Tv: derivative action time (0.0 ... 999.9 min)
ME6	Simulation Off On	Select controller simulation Here, you can switch a configuration loop on or off. The hold is removed with an active controller simulation. Simulation on: The characteristic values entered in the previous field are used in the next field to simulate the controller behaviour. Off: Press "E" to leave the controller simulation.
ME7	Function auto Set: 1000 mS/cm act.: 1000 mS/cm y: 000	Controller simulation Function: Here, you set whether an actuating variable calculated by the controller ("auto"), or an actuating variable y entered by the user ("manual") is to be output. Set: Displays the current setpoint. If necessary, you can change the setpoint. The other points (start/end of neutral zone, optimization points, control points) change accordingly. Actual: Displays the current actual/measured value. Y: With the "auto" function: displays the actuating variable determined by the controller. With the "manual" function, you can enter an actuating variable here. Values < 0 % mean downward dosing, values > 0 % mean upward dosing.

To best adapt the controller parameters to the process, we recommend the following:

- Set values for controller parameter (Field ME5), activate simulation (Field ME6), deflect process: Field ME7: set function to "manual" and enter an actuating variable. Using the actual value, you can observe how the process is deflected.
- Switch the function to "auto". Now you can observe how the controller returns the actual value to the setpoint.
- If you want to set other parameters, press the "Enter" key and you will return to Field ME5. During this time, the controller continues to run in the background.
- If you have made your settings, press the "Enter" key again to return to Field ME6. There, you can continue or exit the simulation.



Note!

Only exit the controller simulation in Field ME6 with "Simulation off". Otherwise, the simulation will continue to run in the background.

6.4.15 Set up 2 – Limit switch

The transmitter has several possibilities for assigning a relay contact. The limit contactor can be assigned an on and off point, as well as a pickup and dropout delay. In addition, an error message can be generated when an alarm threshold is set. You can trigger cleaning in connection with this error message (see error/contact assignment page 49).

These functions can be used both for conductivity/concentration/resistivity measurement and for temperature measurement.

To illustrate the contact states of any relay contact or fault-signalling contact, refer to fig. 31:

On-point > off-point (with increasing measured values):

- The relay contact closes after the on-point at t_1 is exceeded and the pickup delay ($t_2 - t_1$) expires.
- When the alarm threshold at t_3 is reached and the alarm delay ($t_4 - t_3$) also expires, the fault signalling contact switches.
- With returning measured values, the fault-signalling contact reopens when the alarm threshold is undershot at t_5 . The appropriate error message is deleted.
- The relay contact opens again after the off-point is reached at t_6 and the dropout delay has elapsed ($t_7 - t_6$).



Note!

- If the pickup and dropout delays are set to 0 s, the on and off points are the switch points of the contacts.
- You can make identical settings for a minimum function similar to the maximum function.

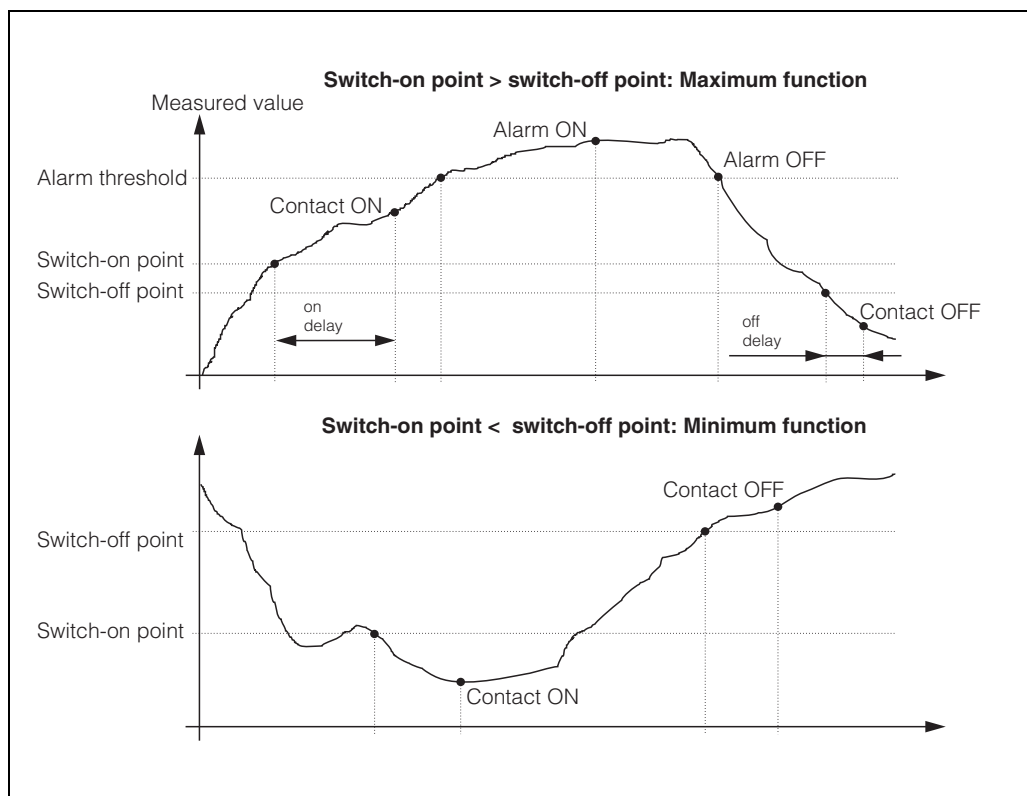


fig. 31: Diagram of the relationship between on and off points and on and off delay

Monitoring of pharmaceutical water according to USP

Mycom S CLM153 with conductive sensors offers a function for monitoring water for injection (WFI) according to the USP (United States Pharmacopeia) standard, part 645.

Measurement is performed as follows:

- The uncompensated conductivity is measured.
- The temperature is measured and the value is rounded down to the next 5 °C step.
- The actual measured value is compared with the limit value for water according to USP at the corresponding temperature (see table).
- If the limit value is exceeded, an alarm is triggered.

Additionally, Mycom S offers a pre-alarm which is triggered at a freely configurable value (e.g. 80 % of USP value). You can use this pre-alarm to start regeneration of your plant in time.




Note!

- The USP function is activated by assigning a limit switch to USP CH1 or USP CH2. The alarm is set via the alarm relay and the error messages E154 to E157. The pre-alarm is set by the relay assigned to the corresponding limit value (see chap. 6.4.5).
- The transmitter always uses uncompensated conductivity values for the USP function even if temperature-compensated values are shown on the display.

Temperature [°C]	Conductivity [µS/cm]	Temperature [°C]	Conductivity [µS/cm]
0	0.6	55	2.1
5	0.8	60	2.2
10	0.9	65	2.4
15	1.0	70	2.5
20	1.1	75	2.7
25	1.3	80	2.7
30	1.4	85	2.7
35	1.5	90	2.7
40	1.7	95	2.9
45	1.8	100	3.1
50	1.9		


To enter the menu, proceed as follows:

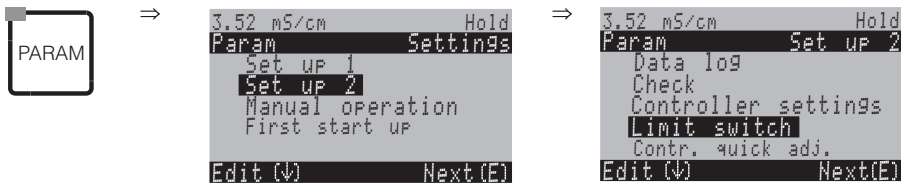

CODE	CHOICE (default = bold)	INFO
O1	Limit switch 1 Limit switch 2 Limit switch 3 Limit switch 4 Limit switch 5	Selection of the limit switch which you wish to configure. There are five limit switches available.
Limit switch 1 / 2 / 3 / 4 / 5:		
OA1 / OB1 / OC1 / OD1 / OE1	Function off Assignment PV CH1 On point: 2000mS/cm / 0500 MΩ·cm / 99.99% / 10.50 pH Off point: 2000mS/cm / 0500 MΩ·cm / 99.99% / 10.50 pH	Limit switch configuration: Function: Activation of function as limit switch 📎 Note! A limit switch can only be activated if a relay has been assigned to it, see chap. 6.4.5. Assignment: Selection of the measured value to which the limit value should apply. Selection: primary value CH1, tem- perature CH1, primary value CH2, temperature CH2, USP CH1, USP CH2 (conductive sensors), combined (only if operating mode = combined circuits) On-point: Entry of the value at which the limit function is activated. Off-point: Entry of the value at which the limit function is deactivated. (Settable range: 0 ... 2000 mS/cm / 0 ... 100% / 0 ... 100 MΩ / -50 ... +150°C / pH = 7.00 ... 11.0)
OA2 / OB2 / OC2 / OD2 / OE2	On delay: 0000 s Off delay: 0000 s Alarm thresh- hold: 2000mS/cm / 500 MΩ·cm / 99.99% / 10.50 pH	Limit switch configuration: On delay: Entry of the switch-on delay of the limit switch relay (range 0 ... 2000 s) Off delay: Entry of the switch-off delay (range 0 ... 2000 s) Alarm threshold: Entry of the value (alarm threshold) at which the fault signalling contact switches.

6.4.16 Set up 2 – Controller quick adjustment

To enter the menu, proceed as follows:

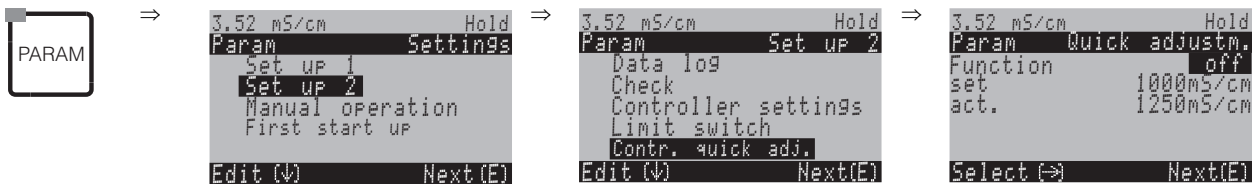

6.4.17 Set up 2 – Chemoclean

Chemoclean[®] is a system to automatically clean conductivity sensors. Water and cleaner are conveyed to the sensor by means of an injector (e.B. CYR10).



Note!

The function group is only active if you have set Chemoclean = on in the "Setup 1" → "Relays" menu; s. Field F1, chap. 6.4.5 page 40.

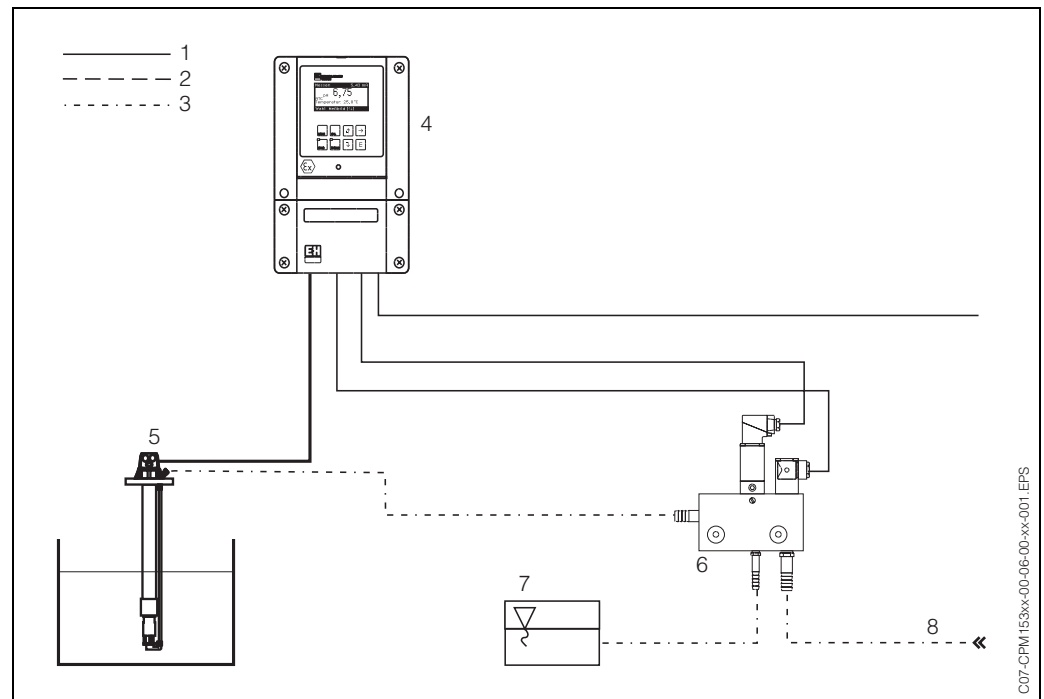


fig. 32: 1: Electric line
2: Pressurised air
3: Water/cleaning liquid
4: CLM153 transmitter
5: Immersion assembly
6: Injector CYR10
7: Cleaning liquid
8: Motive water

Operation:

1. In the menu "Set up 1" → "Relays" (Field F1, s. page 40), the Chemoclean[®] function must be switched on and the appropriate contacts connected to the injector.
2. The cleaning processes are configured in the menu "PARAM" → "Set up 2" → "Chemoclean". Here, the automatic or event-controlled cleaning can be adapted to the process conditions. One or more of the following controls are possible:
 - Weekly programme (see below, Fields OA1 to OAA5): Any number of cleanings can be started on each weekday
 - External control: a start can be triggered via the binary input. For this, external control must be activated in Field P1, "Select control levels": Ext. control "on")
 - Clean trigger: Cleaning is carried out if an error with a cleaning trigger occurs, (see also Field LM1 under "Set up 2" → "Check systems")
 - Power failure: cleaning is started after a power failure.

Manual operation:

Rapid on-site cleaning can be carried out with the menu:
"PARAM" → "Manual operation" → "Chemoclean" → press "E" twice ("start cleaning")

Weekly programming:

"PARAM" → "Set up 2" → "Chemoclean":
Each day can be programmed individually. The following programmes are available

- "Clean": Cleaning started by entering the start time (s. fig. 33).
- "Clean Int": Cleaning is carried out at intervals with a defined spacing (s. fig. 33). This programme cannot be started via the binary inputs directly.
- "User": User-defined cleaning programmes (create in Programme Editor; from Field NAD1).

Programme sequences (cleaning example)

Monday:
2 x cleaning (at 11:00 and at 18:00) with 120 s. water, of which 60 s. additionally with cleaner.
Clean every 30 mins. between 18:20 and 24:00 (= 1800 s.) with 120 s. water, of which 60 s. additionally with cleaner.

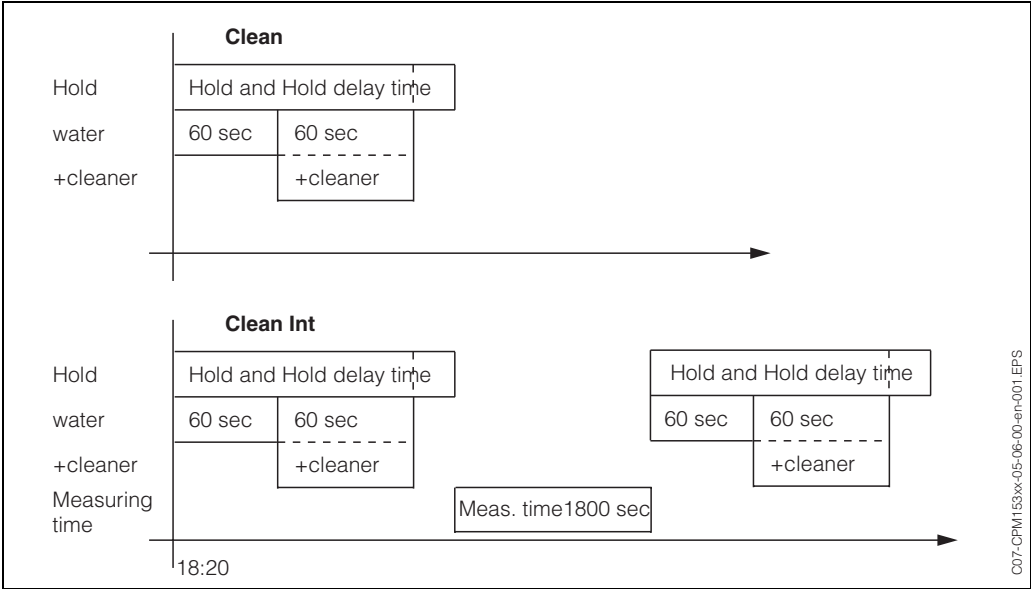



fig. 33: Graphic representation of the above example

Required settings according to the example
(**bold**: to be set by user):

Field OAA1	Field OAA2 (with "Clean")	Field OAA2 (with "Clean Int")
Clean	01 Water 60 s	01 Water 60 s
11:00 11:02	02 +Cleaner 60 s	02 +Cleaner 60 s
Clean	03 Water 0s	03 Water 0s
18:00 18:02	04 Rep. Clean 0x	Measuring time 1800s
Clean Int		
18:20 24:00		

In this way, each day can be programmed (or copied) individually.

To enter the menu, proceed as follows:

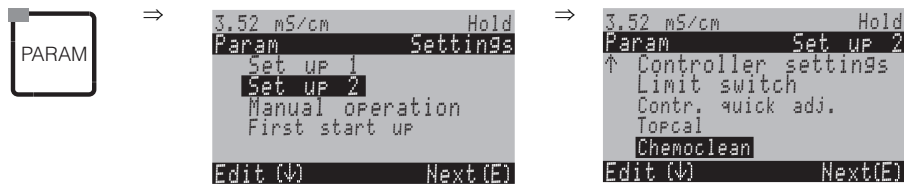


CODE		CHOICE (default = bold)		INFO
P1		Automatic Clean trigger Ext. Control	off off off	Select control levels Activate the function which should trigger Chemoclean cleaning.
P2		Automatic Clean trigger Ext. Control	off off off	Note in display: Displays the current system status
P3		Automatic User prg.		Select the configuration menu Automatic: Here, you can select cleaning programmes for each weekday. User programme: Here you create customer-specific programmes using the Programme Editor (see Programme Editor, p. 76).
	Automatic:			
PA1		Monday Tuesday Sunday	1 2 ... 0	Weekday selection menu Select cleaning day. The number of cleaning triggers for the day is shown behind each day.
PA2		Edit day? Copy day?		Select day function Edit day: You edit the cleaning sequence for this day. Copy day: The day selected in OA1 is copied to the day selected in the field below.
	Edit day:			
	PAA1	Clean 18:22 18:23 No progr.		View/edit day programme You can see the complete daily programme or "No Progr.". You can overwrite the option and also the already set programmes by making a new selection. The start and finish times are always given. Example: Clean 18:22 (start time) 18:23 (finish time) User prog.: Use of a programme you created (see Programme Editor, p. 76)
	PAA2	01 Water 02 +Cleaner 03 Water 04 Rep. cleaning	0 s 30 s 30 s 0x	Select programme blocks The times for individual programme steps can be individually adjusted here. Select a block for editing by pressing "E". +Cleaner: Cleaner is conveyed in addition to water. Rep. cleaning: Number of repetitions of the previous steps 01 ... 03  Note! ■ When you change one of this programme blocks the changes will affect every cleaning. ■ Leave this selection by pressing "PARAM".

CODE		CHOICE (default = bold)	INFO
	PAA3	0010 s (0 ... 9999s)	Water / cleaner: Enter the time during which the valve remains open to allow the conveyance of water or cleaner.
	PAA4	Repeat x number of times 00 (0 ... 10)	Repeat cleaning How often should the previous step (cleaner or water) be repeated?
	Copy day:		
	PAB1	Tuesday Wednesday ... Sunday	? = Monday Select the day to which you want to copy Monday (example).  Note! Danger of data loss. When copying one day to another, the cleaning programmes of the target day are overwritten.
User programme: (Programme Editor)			
	PAB1	User prog. 1	Select user programme With Chemoclean there is one user programme available.
	PAB1	Edit Insert template Enable Disable Rename	Select edit function Insert template: An installed programme (e.g. Clean) can be inserted into the user programme.  Note! ■ After a programme is disabled, it can be re-enabled at any time. ■ Leave this item by pressing "PARAM".
	Edit:		
	PBA1	01 02	Select rows The row with the selected position number can be edited with "E".  Note! Leave this selection by pressing "PARAM".
	PBA2	Change Insert Move to Delete	Select the edit function for the selected block Change: The function is changed for the selected position Insert: A new block is inserted before the highlighted position. Move to: The highlighted function is moved to a different position. Delete: The highlighted function is deleted (there is no query whether you really want to delete!)
	Change / insert:		
	PBAA1	Water +Cleaner Wait Back to ...	Select function Back to: You can create a programme loop with this function (for repeats). Possible selection: Water, +cleaner, wait, back to

CODE		CHOICE (default = bold)	INFO
		Move to:	
	PBAA2	(Displays blocks as list) 01 Water 02 +Cleaner 03 Wait	Select rows You move the function selected in Field NADA1 to the highlighted position.  Note! The highlighted function will be overwritten.
		Insert template:	
	PBB1	User prog. = ? No prog. Clean _____	Select the template you want to copy to the user programme.
		Activate programme:	
	PBC1	Programme is activated	Note in display (no entry): The created or edited programme is enabled.
	PBC2	User prog. (0 ... 9; A ... Z)	Change name 9-character name for your user programme, freely selectable.
		Lock programme	
	PBD1	Do you want to lock the programme?	Query Pressing "E" (= Continue) disables the programme. Pressing "PARAM" (= Cancel) takes you back without disabling the programme.
	PBD2	The programme was locked.	Note in display (no entry)
		Rename programme:	
	PBE1	User prog. (0 ... 9; A ... Z)	Change name 9-character name for your user programme, freely selectable.

6.4.18 Manual operation


To enter the menu, proceed as follows:

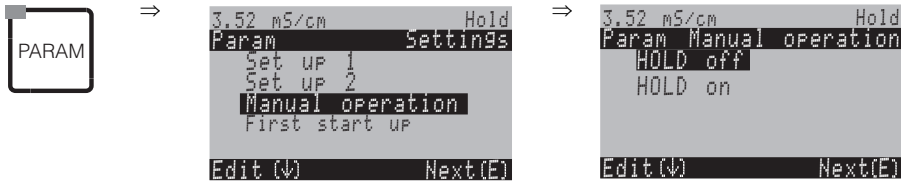

CODE	CHOICE (default = bold)	INFO
R1	Chemoclean Hold	Select manual operation Note! ■ Leave the manual operating menu by pressing "PARAM", "DIAG" or "MEAS". ■ The settings are only active in this menu. Nothing is saved when you leave.
R2	!!!Caution!! You are now leaving manual operation.	If you leave the manual operation: Note in display Confirm by pressing "Enter": Leave the manual operation. Cancel by pressing "PARAM": Continue with manual operation.
Chemoclean:		
RB1	Automatic off Clean trigger off Ext. Control off	Note in display (no entry): System status
RB2	no prog Clean	Chemoclean cleaning No prog: Here, each external programme start is suppressed. Clean: Here, you can start the Clean programme. Note! Leave this item by pressing "PARAM".
HOLD:		
RC1	HOLD off HOLD on	Select manual operation Activate / deactivate Hold The "HOLD" function freezes the current outputs as soon cleaning/calibration is undertaken. Note! If the controller function lies on current output 2, it follows the instructions of the defined "controller hold" (s. page 50).

6.4.19 Diagnosis

To enter the menu, proceed as follows:

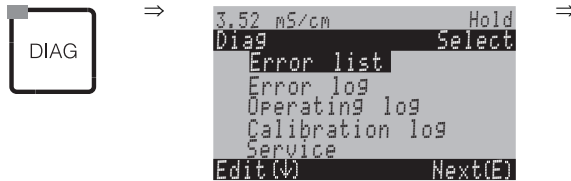

CODE	CHOICE (default = bold)	INFO
U	Error list Error log Operation log Calibration log service	Error list: Displays the current active errors. (Complete error list with description s. page 92) Error log: Lists the last 30 signalled errors with date and time. Operation log (service code necessary): Lists the last 30 registered operating steps with date and time. Calibration log: Lists the last 30 calibrations undertaken with date and time. Note! ■ Use the arrow keys to scroll through the lists. ■ Leave the lists by pressing "E".
Service:		
Y	Factory reset Simulation Instrument check Reset DAT download Instrument version Chemoclean Reset count	Selection for service diagnosis Factory reset: Different data groups can be reset to the factory settings. Simulation: The transmitter behaviour can be simulated after entering various parameters. Instrument check: The instrument functions (display, keys, etc.) can be tested individually. Reset: Device reset ("warm start") DAT download: Copy data into/out of the DAT module. Instrument version: Device internal data e.g. serial number can be queried. Chemoclean (only, if the complete Chemoclean function is activated): Inspecting programmes, inputs, mechanics. Factory function: Reset counter, write access
Factory reset:		
YA1	Abort Only start up data Only calibration data Complete reset Service data Operation log Error log Calibration log	Set default Here you can select the data which you wish to reset to the factory settings. Note! Danger of data loss. Selecting a point and confirming with "Enter" deletes all the settings you made in this area! Pressing Cancel leaves this field without changing the values. Calibration data: All the saved data for calibrations such as zero point, slope, and offset. Start up data: The remaining data to be set. Complete reset: Calibration data + setting data Service data: All data + logbooks + reset counters. Service data / logbooks: These functions are only for authorised service personnel. The service code is required.

CODE		CHOICE (default = bold)	INFO
		Service data / logbooks:	
	YAA1	0000	Entry of the service code required  Note! For service code setting, see Field D1, p. 35.
	YAA2		Note in display: Incorrect service code entry (back to the last field)
	Simulations:		
	YB1	Simulation: off Output 1: 12.00 mA Output 2: 04.00 mA	Adapt simulation (current outputs) Simulation off: The frozen values from the last measurement are used for the simulation. Simulation on: The current values for the outputs can be changed (Output 1, Output 2)
	YB2	Simulation: off PV 1: 1mS/cm Temperature: 025.0 °C PV 2: 0mS/cm Temperature: 000.0 °C	Adapt simulation (measured value/temperature) Simulation off: The frozen values from the last measurement are used for the simulation. Simulation on: The values (measured value/temperature) can be changed.
	YB3	Simulation: off Alarm relay: off Relay 1: off Relay 2: off	Adapt simulation (contacts) Simulation off: The last statuses are frozen and used for the simulation. Simulation on: The contacts can either be opened (on) or closed (off).  Note! If you return to the measurement mode with the simulation switched on, "Simul" and "Hold" flash in the display.
	Instrument check:		
	YC1	Display Keypad RAM EEPROM Flash	Selection for check Display: All the fields are queried alternately. Defective cells become visible. Keypad: All the keys must be pressed one after the other. If the system is functioning perfectly, the appropriate symbols appear in the display. RAM: "RAM O.K" message if there are no errors. EEPROM: "EEPROM O.K" message if there are no errors. Flash (memory): "Flash OK" message if there are no errors.  Note! Leave this item by pressing "PARAM".

CODE		CHOICE (default = bold)	INFO
		DAT download (only available if DAT module is plugged in):	
	YD1	DAT write DAT read Erase DAT	DAT selection DAT write: You can save the both the configuration and the logbooks of your transmitter to the DAT module. DAT read: Copy the configuration saved on the DAT module into the EEPROM of the transmitter. Erase DAT: Delete all data on the DAT module.  Note! After the "DAT read" copying procedure, a reset is triggered automatically, and the device is configured with the copied values. (See below for reset).
		DAT write:	
	YD2	!!Caution!! All the data on the DAT module will be deleted.	Note in display For safety reasons, you are asked if you really want to overwrite the existing data.
	YD3	in process	Data are written to the DAT module
		DAT read:	
	YD4	!!Caution!! All the data in the Mycom S will be deleted.	Note in display For safety reasons, you are asked if you really want to overwrite the existing data.
	YD5	in process	Data are written to Mycom S
		Erase DAT:	
	YD6	!!Caution!! All the data on the DAT module will be deleted.	Note in display For safety reasons, you are asked if you really want to delete the existing data.
		Reset	
	YE1		Reset You can restart the Mycom S with this function (similar to the "warm start" on your computer). You can use this function if the Mycom S does not react as expected.  Note! This reset does not change saved data.
		Instrument version:	
	YF1	SW Version: 1.2 HW Version: 1 Serial No.: 12345678 Card ID: A1B	Controller data Open controller data and the hardware version.
	YF2	SW Version: 1.2 HW Version: 1 Serial No.: 12345678 Card ID: A1B	Basic module data
	YF3	SW Version: 1.2 HW Version: 1 Serial No.: 12345678 Card ID: A1B	Transmitter 1 data Open transmitter data (1).

CODE		CHOICE (default = bold)	INFO
	YF4	SW Version: 1.2 HW Version: 1 Serial No.: 12345678 Card ID: A1B	Transmitter 2 data Open transmitter data (2).
	YF5	SW Version: 1.2 HW Version: 1 Serial No.: 12345678 Card ID: A1B	DC-DC converter data (only for two circuit)) Module for power supply of transmitter 2
	YF6	SW Version: 1.2 HW Version: 1 Serial No.: 12345678 Card ID: A1B	Relay data
	YF6	12345678901234	Enter serial number 14 digit number consisting of 0 ... 9 and A ... Z
	YF7	CLM153-A2B00A010	Order Code 15 digit number consisting of 0 ... 9 and A ... Z
	Chemoclean:		
	YH1	Automatic off Clean trigger off Ext. Control off	Note in display (no entry): System status
	YH2	With E running programme is aborted.	Note in display (no entry): To be able to carry out the diagnosis, you must abort the programme currently running by pressing the "Enter" key.
	YH3	Ext. Inputs Mechanics	Selection Chemoclean diagnosis
	Ext. Inputs:		
	YHA1	Start Userprog Auto stop On Wait trigger On Ass. measurement On Ass. service On	Info field: status of external digital inputs
	Hardware:		
	YHB1	Water Cleaner Water and cleaner	Select mechanics Select a function which shall be tested.
	YHB2	Automatic off Clean trigger off Ext. Control off	Note in display (no entry): System status
	Reset count:		
	YI1	0	Reset count (only triggered by watchdog) Can be reset via Set Default → service data.
	YH2	0	Write count Number of write accesses to the EEPROM is reported here.

6.4.20 Calibration

The calibration can be protected with the maintenance and the specialist codes. No calibration can be carried out at the display level (compare with page 35).

Procedure:

1. Move assembly to service position (when a retractable assembly is used).
2. Remove sensor.
3. Clean sensor before calibration.

Calibration can be performed in two different ways:

- By measuring with a known conductivity (Fields xx to yy) in a calibration solution
- By entering the precise cell constant of the conductivity sensor (Field A5, p. 33).




Note!

- For the calibration described below, the transmitter must be in "Conductivity" operating mode. If the transmitter shows the resistivity or concentration mode, you have to switch to conductivity mode throughout calibration.
- If automatic temperature compensation is selected for calibration (s. page 28), the corresponding temperature sensor must also be immersed in the calibration solution.
- The instrument switches automatically to Hold (factory setting) whenever it is calibrated.
- Cancel calibration by pressing the "MEAS" key.



```
3.52 mS/cm
Cal      Cancel Calib.
no
yes, Cancel Calib.
Edit (F)  Next (E)
```

- If you confirm this with "yes, cancel cal.", you return to the measurement mode.
- If you select "no", calibration is continued.

To enter the menu, proceed as follows:

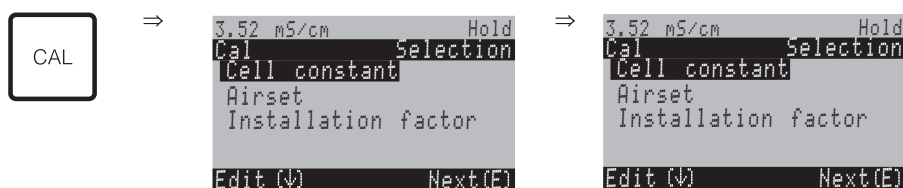

CODE	CHOICE (default = bold)	INFO
C1	Sensor 1 Sensor 2 End calibration	Selection for calibration (only two circuit) Select sensor 1 or 2, and then run through calibration for each individual sensor.
C2	Cell constant Airset Installation factor	Selection Cell constant: Calculate the cell constant of the sensor. Airset (only inductive): The sensor must be calibrated at air and in a dry state. The airset of inductive sensors is performed before determination of the cell constant. Installation factor (only inductive): Sensor calibration with compensation for the wall effect after determination of the cell constant.
Cell constant:		
Note! Below you find a description of a calibration with the temperature-compensated conductivity value of the reference solution. If you want to perform a calibration with uncompensated conductivity, set the temperature coefficient α to zero.		
Immerse the sensor (inductive or conductive) into the calibration solution. Note! Immerse the sensor in such a way that there is a minimum distance of 15 mm to the vessel wall, so that the installation factor does not play a role.		
CB1	025.0 °C (-35.0 ... 250 °C)	Entry of MTC temperature Enter the temperature at which the calibration is performed (only MTC - manual temperature entry).
CB2	2.10 % / K (0.00 ... 20.00 % / K)	Alpha value (TC value) Enter the α value of the calibration solution. This value is specified for the Endress+Hauser calibration solutions or is calculated from the imprinted table
CB3	Current measured value (0.0 ... 9999 mS/cm)	Current measured value Enter the correct conductivity value of the calibration solution. It makes sense to use a calibration solution which is at >40 % of the measuring range of the sensor used. The display is always in mS/cm.
CB4	5.9 cm-1 (0.1 ... 9.99 cm-1)	Cell constant The calculated cell constant is displayed and applied to Field A5 (s. page 33).

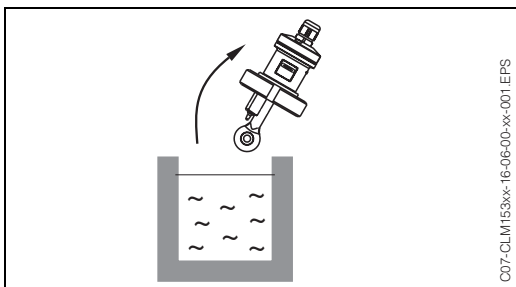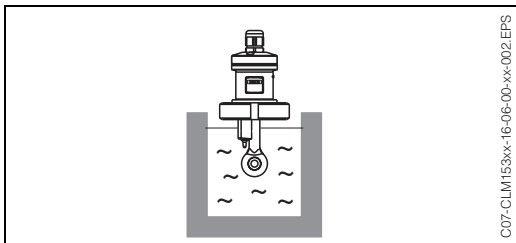CODE		CHOICE (default = bold)	INFO
	CB5	ok	Calibration status
	CB6	Accept Reject Recalibrate	End of calibration Accept: Pressing "E" accepts the new calibration data. Reject: The data are not accepted, a recalibration will not be started. Recalibrate: The data are rejected and a new calibration will be started.
		Proceed with 	
Airset (only inductive):			
		Remove sensor from the liquid and dry thoroughly .  Note! As long as the sensor is out of the medium during Airset, an error code referring to measuring range violation (E055/E056) can be ignored.	 C07-CLM153xx-16-06-00-xx-001.EPS
CA1		0.0µS/cm	Current measured value Start calibration residual coupling using CAL key.
CA2		42µS/cm	Residual coupling The residual coupling of the system (sensor and transmitter) is displayed. (Range: -80 ...80 µS • cell constant)
CA3		ok	Calibration status
CA4		Accept Reject Recalibrate	End of calibration Accept: Pressing "E" accepts the new calibration data. Reject: The data are not accepted, a recalibration will not be started. Recalibrate: The data are rejected and a new calibration will be started.
		Proceed with 	
Installation factor (only inductive):			
		The sensor remains in the place of application.	 C07-CLM153xx-16-06-00-xx-002.EPS
CC1		025.0 °C (-35.0 ... 250 °C)	Entry of MTC temperature Enter the temperature at which the calibration performed (only MTC - manual temperature entry).

CODE	CHOICE (default = bold)	INFO
CC2	2.10 % / K (0.00 ... 20.00% / K)	Alpha value (TC value) Enter the α value of the calibration solution. This value is specified for the Endress+Hauser calibration solutions or is calculated from the imprinted table
CC3	Current measured value (0.0 ... 9999 mS/cm)	Current measured value Enter the correct conductivity value of the calibration solution. It makes sense to use a calibration solution which is at >40 % of the measuring range of the sensor used. The display is always in mS/cm.
CC4	1 (0.10 ... 5.00)	Installation factor The calculated installation factor is displayed and applied to Field AA2 (s. page 33).
CC5	Accept Reject Recalibrate	End of calibration Accept: Pressing "E" accepts the new calibration data. Reject: The data are not accepted, a recalibration will not be started. Recalibrate: The data are rejected and a new calibration will be started.
	Proceed with E	

7 Maintenance

The transmitter Mycom S CLM153 itself does not contain wear parts and is maintenance free. Measuring point maintenance comprises:

- Cleaning of assembly and sensor
- Inspecting cables and connections
- Calibration (s. page 83)



Warning!

Danger to persons. If you have to remove the sensor for servicing or calibration work, pay attention to the hazards caused by pressure, temperature and contamination.



Caution!

Remember that any maintenance work on the instrument, assembly or sensors may have impacts on process control and the process itself.

7.1 Maintaining the measuring system

7.1.1 Cleaning

Depending on the process, and as far as necessary, the assembly, cables and sensor must be cleaned externally before inspection and calibration. For your own safety always follow the safety instructions (see above). If necessary wear protective clothing.

Remove dirt and deposits:

The selection of cleaning agent depends on the type of soiling. The most frequent soiling and the associated cleaning agents are listed in the table below:

Type of soiling	Cleaning agent
Greases and oils	Substances containing tensides (alkaline) or water-soluble organic solvents (e.g. alcohol)
 Warning! Danger of caustic burns! Protect your hands, eyes and clothing when you use the following detergents.	
Calciferous deposits, metal hydroxide deposits, heavy biological deposits Light biological deposits	3% HCl or with Chemoclean: HCl (10%) in injector thinned to approx. 3%
Sulphide deposits	Mixture of hydrochloric acid (3%) and thiocarbamide (commercially available)
Protein deposits	Mixture of hydrochloric acid (0.1 molar) and pepsin (commercially available)
Light biological deposits	Water under pressure

7.1.2 Inspecting cables and connections

Please check cables and connections using the following checklist. As there are many different combination possibilities, these instructions are kept to a general level and must be applied to the current installation.

- Check the sensor plug-in head for airtightness and humidity.
- Check the sensor cable and particularly the outer insulation for breaks.
- Sensor cables which have become damp on the inside must be replaced.
Drying alone is not sufficient!
- If you are using a junction box: The inside of the box must be clean and dry. Moist dehydrating bags must be replaced.*
- Retighten the terminals in the junction box.*
- For field instruments:
Retighten the terminals in the instrument. Also check that the interior and the PCBs are clean, dry and free of corrosion (if not, check the seals and threaded joints for leaks and breaks). *, **
- For panel-mounted instruments:
Retighten the terminals on the instrument, check the BNC connector. *, **
- Cable screens must be connected exactly as shown in the wiring diagram. If the screen is connected incorrectly or not at all, the fail-safety of the instrument could be impaired.

*: The frequency of these checks is dependent on environmental influences. In a normal climate and non-aggressive environment, an annual check is sufficient.

**: This work may only be carried out on a voltage-free instrument, as some of the terminals carry mains voltage.

7.1.3 Simulation of conductive sensors for device test

You can check the transmitter for conductive conductivity by substituting resistors for the measurement section and temperature sensor. The accuracy of the simulation depends on the accuracy of the resistors.

Temperature

The temperature values in the table on the right apply if a temperature offset is not set at the Mycom S.

All resistance values are increased by factor 10 for temperature sensor type Pt 1000.

 Note!

- Connect the temperature equivalent resistor in three-wire technology.
- You can use the service kit "Cond. test adapter" (Order No.: 51500629) when connecting resistor decades instead of the cond. sensor.

Pt 100 equivalent resistances:

Temperature	Resistance value
-20 °C	92.13 Ω
-10 °C	96.07 Ω
-0 °C	100.00 Ω
10 °C	103.90 Ω
20 °C	107.9 Ω
25 °C	109.73 Ω
50 °C	119.40 Ω
80 °C	130.89 Ω
100 °C	138.50 Ω
200 °C	175.84 Ω

Conductivity

If the cell constant k is set to the value in the second column of the table on the right, then the conductivity values of this table apply. Otherwise the following applies: Conductivity $_{[mS/cm]} = k \cdot 1 / R_{[k\Omega]}$

Resistance R	Cell constant k	Display with conductivity
10 Ω	1 cm-1	100 mS/cm
	10 cm-1	1000 mS/cm
100 Ω	0.1 cm-1	1 mS/cm
	1 cm-1	10 mS/cm
	10 cm-1	100 mS/cm
1000 Ω	0.1 cm-1	0.1 mS/cm
	1 cm-1	1 mS/cm
	10 cm-1	10 mS/cm
10 k Ω	0.01 cm-1	1 μ S/cm
	0.1 cm-1	10 μ S/cm
	1 cm-1	100 μ S/cm
	10 cm-1	1 mS/cm
100 k Ω	0.01 cm-1	0.1 mS/cm
	0.1 cm-1	1 μ S/cm
	1 cm-1	10 μ S/cm
1 M Ω	0.01 cm-1	0.01 μ S/cm
	0.1 cm-1	0.1 μ S/cm
	1 cm-1	1 μ S/cm
10 M Ω	0.01 cm-1	0.001 μ S/cm
	0.1 cm-1	0.01 μ S/cm

7.1.4 Simulation of inductive sensors for device test

An inductive sensor alone cannot be simulated using resistors. However, you can use equivalent resistors to check the entire system CLM153 (inductive) including the sensor. Please pay attention to the cell constant k (e.g. $k_{\text{nominal}} = 2$ for CLS50, $k_{\text{nominal}} = 5.9$ for CLS52).

For an exact simulation, use the cell constant actually used (can be read off in Field C124) for calculating the reading:

$$\text{Display cond.}_{[mS/cm]} = k \cdot 1 / R_{[k\Omega]}$$

Reference values for the simulation CLS52 at 25 °C:	Simulation resistance R	Cell constant k	Display cond.
Carrying out the simulation: Guide a line through the opening of the sensor and connect it to a resistor decade, for example.	6.8 Ω	5.90 cm-1	868 mS/cm
	33 Ω	5.90 cm-1	178.8 mS/cm
	330 Ω	5.90 cm-1	17.88 mS/cm
	3.3 k Ω	5.90 cm-1	1.788 mS/cm

7.1.5 Checking conductive conductivity sensors

- Measuring surface connection:
The measuring surfaces are directly connected with connections of the sensor plug. Check with ohmmeter at $< 1 \Omega$.
- Measuring surface shunt:
A shunt may not exist between the measuring surfaces. Check with ohmmeter at $> 20 M\Omega$.
- Temperature sensor shunt:
A shunt may not exist between the measuring surfaces and the temperature sensor. Check with ohmmeter at $> 20 M\Omega$.
- Temperature sensor
Refer to the sensor nameplate for the type of temperature sensor used.
The sensor can be checked with an ohmmeter at the sensor plug:
 - Pt 100 at $25^\circ\text{C} = 109.79 \Omega$
 - Pt 1000 at $25^\circ\text{C} = 1097.9 \Omega$
 - NTC 10k at $25^\circ\text{C} = 10 k\Omega$
- Connection:
Make sure the terminals are correctly assigned for sensors with terminal connection (CLS12/13).
Check that the terminal screws are secure.

7.1.6 Checking inductive conductivity sensors

The following data apply to sensors CLS50 and CLS52.

- Test send coil and receive coil (white and red coaxial cable, each measured between inner connector and screen):
 - ohmic resistance approx. $0.5 \dots 2 \Omega$
 - Inductance approx. $180 \dots 500 \text{ mH}$ (at 2 kHz , serial connection as equivalent circuit diagram)
CLS50: approx. $250 \dots 450 \text{ mH}$
CLS52: approx. $180 \dots 360 \text{ mH}$
- Test coil shunt:
A shunt may not exist between the coils (from red coax to white coax). Check with ohmmeter at $> 20 M\Omega$.
- Test temperature sensor:
You can use the table in chap. 7.1.3 to check the Pt 100. The resistance values between the green and white cores and green and yellow cores must be identical.
- Test temperature sensor shunt:
Shunts may not exist between the temperature sensor (green, white or yellow lines) and the coils (red coax or white coax). Check with ohmmeter at $> 20 M\Omega$.

7.1.7 Checking line extension and boxes

- Use the methods described in chap. 7.1.3 or chap. 7.1.4 to carry out a quick functional check from the sensor plug (for conductive sensors) or from the sensor (for inductive sensors) to the device. The easiest way to connect the resistor decades is with the "conductivity test adapter" service kit, Order No: 51500629.
- Check the junction boxes for:
 - moisture (impact at low conductivity, if necessary dry box, replace seals, insert dehydrating bag)
 - correct connection of all lines
 - connection of the outer screening
 - security of the terminal screws.

8 Troubleshooting

Trouble-shooting relates not only to measures which

- can be carried out without opening the instrument but also
- to instrument defects which require the replacement of components.

8.1 Troubleshooting instructions

In this chapter, you will find diagnosis information and information on eliminating errors which occur:

- chap. 8.1.1, p. 92: Error number list → List of all occurring error numbers.
- chap. 8.1.2, p. 95: Process-specific errors → e. g. temperature value is incorrect.
- chap. 8.1.3, p. 97: Device-specific errors → e. g. display is dark.

Before starting the repair work, please note the following safety instructions:



Warning!

Danger to life.

- De-energise the instrument before you open it. Check that there is no voltage and secure the switch(es) against switch-on.
- If work is required under voltage, this may only be carried out by an electrician, but a second person must be present for safety reasons.
- Switching contacts may be powered by separate circuits. Also de-energise these circuits before you work on the terminals.



Caution!

Danger to components through electrostatic discharge (ESD).

- Electronic components are sensitive to electrostatic discharge. Take protective measures, e.g. remove the charge from your person by touching the PE or wear a permanent grounding in the form of a wrist strap.
Highly dangerous: Plastic floors at low air humidity and clothing made of synthetic materials.
- For your own safety, always use genuine spare parts. Only genuine spare parts ensure the correct function, accuracy and reliability after repairs.


8.1.1 Error number list: Troubleshooting and configuration

In the following error list, you can find a description of all the error numbers occurring.

For each error number there is also data on whether the factory setting (= Fact.) of this error triggers

- an alarm,
- an error current or
- cleaning.

To enter the error list, proceed as follows:

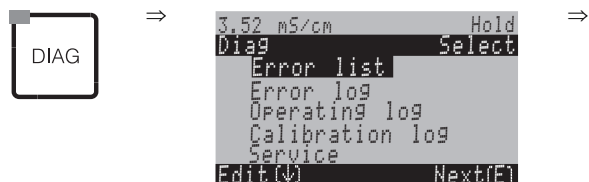

Note!

- Please process the errors as shown in Field H5 (Alarm menu) on page 49.
- The second column shows the assignment acc. to NAMUR work sheet NA64 (failure, maintenance, function control).

Error no.	NAMUR class	Error message	Possible causes / measures	Alarm contact		Error current		Automatic cleaning start	
				Fact.	User	Fact.	User	Fact.	User
E001	Failure	Memory error	Switch instrument off and back on. Corrective maintenance in the factory, if necessary.	yes		no		–	–
E002	Failure	Data error in EEPROM		yes		no		–	–
E003	Failure	Invalid configuration							
E004	Failure	Incompatible hardware	The new software cannot recognise the module.						
E006	Failure	Error transmitter 2	Test with new transmitter.	yes		no		–	–
E007	Failure	Error transmitter 1		yes		no		–	–
E008	Failure	Error sensor 1	Check sensor and sensor connection (chap. 7.1.5 / chap. 7.1.6 or by Endress+Hauser service)	yes		no		no	
E009	Failure	Error sensor 2		yes		no		no	
E010	Failure	Error temp. sensor 1	Check temperature sensor and connections; if necessary, check transmitter with temperature simulator.	yes		no		no	
E011	Failure	Error temp. sensor 2		yes		no		no	
E019	Failure	Delta limit exceeded	Check single measured values (input 1 / input 2) for plausibility	yes		no		–	–
E025	Failure	Limit Airset Offset 1 exceeded	Carry out airset again (only inductive; at air) or replace sensor. Clean and dry sensor before airset.						
E026	Failure	Limit Airset Offset 2 exceeded							
E034	Failure	Calibrating range of measuring cell 1 exceeded	Clean sensor and recalibrate; if necessary, check sensor, line and connections.	yes		no		–	–
E035	Failure	Calibrating range of measuring cell 1 under range		yes		no		–	
E036	Failure	Calibrating range of measuring cell 2 exceeded		yes		no		–	
E037	Failure	Calibrating range of measuring cell 2 under range		yes		no		–	
E038	Maintenance	Delta limit exceeded	Check single measured values (input 1 / input 2) for plausibility Measuring can still continue until failure error E019 occurs.	yes		no		–	–

Error no.	NAMUR class	Error message	Possible causes / measures	Alarm contact		Error current		Automatic cleaning start	
				Fact.	User	Fact.	User	Fact.	User
E046	Failure	Installation factor range of measuring cell 1 exceeded	Check pipe diameter, clean sensor and carry out calibration again (only for inductive).						
E047	Failure	Installation factor range of measuring cell 1 under range							
E048	Maintenance	Installation factor range of measuring cell 2 exceeded		yes		no		–	–
E049	Maintenance	Installation factor range of measuring cell 2 under range		yes		no		–	–
E053	Failure	Actuator failure							
E054	Maintenance	Dosing time alert	Feedback to controller defective	yes		no		–	–
E055	Failure	Display / measuring range of main measured value 1 under range	Immerse sensor in conductive medium. For inductive: Carry out airset. As long as the sensor is out of the medium during Airset, an error code referring to measuring range violation can be ignored.	yes		no		no	
E056	Failure	Display / measuring range of main measured value 2 under range		yes		no		no	
E057	Failure	Display / measuring range of main measured value 1 exceeded		yes		no		no	
E058	Failure	Display / measuring range of main measured value 2 exceeded		yes		no		no	
E059	Failure	Temperature 1 under range	Temperature sensor defective; Sensor line interrupted or short-circuited; Incorrect sensor type selected Simulation s. chap. 7.1.3 / chap. 7.1.4.	yes		no		no	
E060	Failure	Temperature 2 under range		yes		no		–	–
E061	Failure	Temperature 1 over range		yes		no		no	
E062	Failure	Temperature 2 over range		yes		no		–	–
E063	Failure	0/4 mA limit output 1	Measured value outside specified current range: Check measured value for plausibility, if necessary adjust current output assignment 0/4 mA and/or 20 mA.	yes		no		no	
E064	Failure	20 mA limit output 1 exceeded		yes		no		no	
E065	Failure	0/4 mA limit output 2		yes		no		–	–
E066	Failure	20 mA limit output 2		yes		no		–	–
E067	Maintenance	Alarm threshold of limit switch 1 exceeded	Dosing devices defective; chemical supply empty; measured value incorrect → check for plausibility and function; Incorrect control direction set; incorrect contact assigned; Incorrect control function assigned	yes		no		–	–
E068	Maintenance	Alarm threshold of limit switch 2 exceeded		yes		no		–	–
E069	Maintenance	Alarm threshold of limit switch 3 exceeded		yes		no		–	–
E070	Maintenance	Alarm threshold of limit switch 4 exceeded		yes		no		no	
E071	Maintenance	Alarm threshold of limit switch 5 exceeded		yes		no		no	
E072	Failure	Polarisation 1	Clean sensor. Use higher cell constant.						
E073	Failure	Polarisation 2		yes		no		no	
E074	Failure	Temperature 1 out of range of TC table	Check measurement and tables for plausibility; if necessary, adjust or extend table.	yes		no		no	
E075	Failure	Temperature 1 out of range of conc. table		yes		no		no	
E076	Failure	Conductivity out of range of conc. table		yes		no		no	

Error no.	NAMUR class	Error message	Possible causes / measures	Alarm contact		Error current		Automatic cleaning start	
				Fact.	User	Fact.	User	Fact.	User
E077	Failure	Temperature 2 out of range of TC table	Check measurement and tables for plausibility; if necessary, adjust or extend table.						
E078	Failure	Temperature 2 out of range of conc. table							
E079	Failure	Conductivity 2 out of range of conc. table							
E080	Funct. check	Range of current output 1 too small	Increase measuring range span for current output assignment	no		no		no	
E081	Funct. check	Range of current output 2 too small		no		no		no	
E091	Failure	Display / measuring range combined value below range	combined pH value < 7 pH	yes		no		no	
E092	Failure	Display / measuring range combined value above range	combined pH value > 11 pH	yes		no		no	
E100	Funct. check	Current out simulation on	Check if functions were consciously selected	no		no		no	
E101	Funct. check	Service function on		no		no		no	
E106	Funct. check	Download active	Wait for download to end.	no		no		no	
E116	Failure	Download error	Repeat download.	no		no		no	
E117	Failure	Error DAT module	Check with other DAT memory module; when writing to DAT: repeat write process	yes		no		–	–
E152	Maintenance	PCS 1 alarm	Conductivity sensor defective or totally soiled; measured water flow in bypass interrupted; air cushion in assembly; measuring line interrupted	no		no		no	
E153	Maintenance	PCS 2 alarm		no		no		no	
E154	Maintenance	Error USP 1	Conductivity too high, check process. Check temperature for plausibility.	no		no			
E155	Maintenance	USP 1 temperature error		no		no			
E156	Maintenance	Error USP 2		no		no		no	
E157	Maintenance	USP 2 temperature error		no		no			
E171	Maintenance	Current input 1 under range	Measure input signal. Permitted: 4 ... 20 mA Resistance input: see controller configuration (feedback) also	no		no			
E172	Maintenance	Current/resistor input 1 over range		no		no			
E173	Maintenance	Current input 2 under range	Cause is the connected device or the wiring.	no		no			
E174	Maintenance	Current input 2 over range		no		no			

8.1.2 Process-specific errors

Error	Possible cause	Remedial action	Equipment needed, spare parts
Instrument unconfigurable, Display for code prompt is 9999	Instrument hardware is locked via keypad (Keys "CAL" + "DIAG" simultaneously = security locking)	Press "MEAS" and "PARAM" simultaneously to unlock.	
Permanent, incorrect measured value	Sensor does not immerse completely Air cushion in assembly Earth fault at or in the instrument Instrument in impermissible operating state (no response on pressing key)	Check installation position Check assembly and installation position Test measurement in insulated vessel, possibly with calibration solution Switch instrument off and on	Plastic vessel, calibration solutions. Behaviour, when instrument is connected to process? EMC problem: If repeated, check grounding and wire routing
Incorrect temperature reading	Incorrect sensor connection Measuring cable defective Incorrect sensor type selected Sensor defective	Check connections using wiring diagram Check cable Set sensor type on instrument (Field 141) Check sensor	Wiring diagram s. chap. 4.1.1 Ohmmeter Check temperature sensor with Ohmmeter.
Measured values fluctuate	Interference in measuring cable Faults in signal output line	Connect cable screens as per terminal diagram Check line installation, possibly route line separately.	Wiring diagram s. chap. 4.1.1
Div. controller, timer or clean functions cannot be activated	Relay module not available for relay 3 - 5	Install 3 relay module M3R-3	Order number and installation s. page 99.
Controller / limit contact does not work	Controller switched off Controller in "Manual / Off" mode Pick-up delay setting too long "Hold" function active "Auto hold" during calibration "Hold" input activated Manual "hold" active using keypad "Hold" active during configuration	Activate controller s. chap. 6.4 Select "Auto" or "Manual on" mode. Switch off or shorten pick-up delay period Determine cause of hold and eliminate if not desired	Keypad / PARAM / manual operation / contacts "Hold" is indicated in display when active
Controller / limit contact work continuously	Contact in "Manual/on" mode Dropout delay setting too long Control circuit interrupted	Set controller to "Manual/off" or "Auto". Shorted dropout delay period Check measured variable, current output or relay contacts, actuators, chemical supply	
No conductivity/mV current output signal	Line open or short-circuited Output defective	Disconnect both (!) lines and measure directly on instrument Replace controller module	mA meter 0–20 mA DC
Fixed current output signal	Current simulation active Processor system inactive "Hold" is active.	Switch off simulation Switch instrument off and on "Hold" status see display.	s. DIAG / Service / Simulation EMC problem: If repeated, check installation
Current output signal incorrect or different than expected	Incorrect current assignment Incorrect signal assignment Total load in current circuit too high (> 500 ohms)	Check current assignment: 0–20 mA or 4–20 mA selected? Any current output can be assigned to any measured value (conduct. 1 or 2, temp. 1 or 2, characteristic value) Disconnect output and measure current directly on instrument	Check under "PARAM" / current output. mA Meter for 0–20 mA DC

Error	Possible cause	Remedial action	Equipment needed, spare parts
Feed forward control does not work	Additional module M3R-x missing Incorrect version	Additional module M3R-2I with 1 or M3R1I with 2 current inputs	See spare parts list in chap. 8.3 Resistance input only permissible with non-Ex.
Feedback input does not work	Additional module M3R-x missing		See spare parts list in chap. 8.3 Resistance input only permissible with non-Ex.
Feedback incorrect	Feedback potentiometer outside range Feedback range not set or not set correctly	Smallest permissible potentiometer 1 kOhm, largest permissible potentiometer 10 kOhms Set lower and upper range value in "PARAM" menu	
Feedback varies	Connecting cable in non-screened version Cable screening not applied to transmitter. Feedback cable is parallel to h.c. power line (inductive coupling).	Replace cables with screened cables. Apply cable screening to PE rail. Apply cable screening on PE, both sides.	
Data cannot be saved	No DAT memory module available		DAT available as accessory, s. chap. 9

8.1.3 Instrument-specific errors

Error	Possible cause	Tests and / or remedial action	Equipment, spare parts, personnel
Display dark, no LEDs active	No mains voltage Incorrect supply voltage or too low Connection defective Instrument fuse defective (non-Ex) Power unit defective Central module defective (if all 6 LEDs on the power unit are lit) Ribbon cable loose or defective	Check whether mains voltage is applied Compare actual mains voltage with nameplate data Terminal not picked-up; insulation clamped Replace fuse after comparing mains voltage and nameplate data Replace power unit, pay attention to variant Replace central module pay attention to variant Check ribbon cable	Electrician / e.g. multimeter Electrician / correct fuses; s. drawings in chap. 8.7 On-site diagnosis: all 6 red LEDs on the M3G module must be lit On-site diagnosis by E+H Service (test module required) Cable soldered onto the site of the M3G module
Display dark, but LED active	Central module defective (Module: M3Cx-x)	Replace central module M3Cx-x	On-site diagnosis by Endress+Hauser service (test module required)
Display functioning, but not change in display and/or instrument cannot be operated	Instrument or module in instrument not correctly installed Operating system in impermissible state	Check module connections Switch instrument off and on	See device view on page 100 Possibly EMC problem: if problem persists, have installation checked by E+H Service
Instrument gets hot	Incorrect mains voltage or too high Power unit defective	Compare mains voltage and nameplate data Replace power unit	all 6 red LEDs on the M3G module must be lit
Incorrect conductivity measured value / and / or temperature measured value	Transmitter module defective (module: MKIC), first carry out tests and take measures as per chap. 8.1.2.	Test measuring inputs: Connect resistors as per simulation tables p. 89/p. 89 and check display. Temp.: Resistance 100 Ω (for pt 100) of terminals 11 to 12+ 13. Display must be 0 °C	If test negative: Replace module MKIC, bushing using the device view on page 100
Current output, Current value incorrect	Calibration incorrect Load too high Shunt / short-circuit to frame in current circuit Incorrect operating mode	Test with integrated current simulation, connect mA meter directly to current output Check, whether 0–20 mA or 4–20 mA is selected	If simulation value incorrect: new module M3Cx-x required. If simulation value correct: check current circuit for load and shunts
No current output signal	Current output stage defective (Module: M3CH-x) Instrument with PROFIBUS® interface	Test with integrated current simulation, connect mA meter directly to current output PROFIBUS® instruments do not have a current output	If test negative: Replace module M3CH-x (Check variants, see spare parts list in chap. 8.3) For information, see "DIAG" / instrument version

8.2 Response of outputs to errors

8.2.1 Response of current outputs

If an error occurs in the system, an error current is output at the current outputs. You can adjust the value of this error current in the Alarm menu (see page 49).

If you have configured the controller for functioning with a current output, no error current is output on this current output should an error occur.

8.2.2 Response of contacts to errors

You can select the assignment of which instrument error messages trigger an alarm individually for each error message, (see table on page 92, editing errors on page 49). In "NAMUR" mode, failure messages (E 001 – E 029) always trigger an alarm.

Behaviour with standard setting

Instrument status	Alarm relay	Limit value / Controller
Normal operation	picked-up (Fail-safe behaviour)	Appropriate configuration and operating status
Alarm	Dropped out	
Voltage-free	Dropped out	Dropped out

Behaviour with NAMUR setting (contacts configured as active open contacts)

Instrument status	Alarm relay	Maintenance relay	Function check	Limit value / Controller
Normal operation	Picked up (Fail-safe behaviour)	Picked up	Picked up	Appropriate configuration and operating status
Failure	Dropped out	Picked-up	Picked up	Appropriate configuration and operating status
Maintenance required	Picked up	Dropped out	Picked up	Appropriate configuration and operating status
Function check	Picked up	Picked-up	Dropped out	Appropriate configuration and operating status
Voltage-free	Dropped out	Dropped out	Dropped out	Dropped out

8.2.3 Response of contacts to power failure

In the "Set up 1" menu → "Relays", you can define the contacts as active open contacts or active closed contacts (s. page 40). In the case of a power failure, the contacts will act according to the setting you make.

8.3 Spare parts

For your own safety, always use genuine spare parts. Only genuine spare parts ensure the correct function, precision and reliability after repair.

You receive all spare parts in the form of service kits with a unique code, optimally adapted packaging including ESD protection for modules and a set of instructions.

Spare parts list

No.	Kit name	Contents / Use	Order code
10	Terminal module non-Ex	Module M3K	51507084
30	Power supply 100 ... 230 VAC non-Ex	Module M3G, power unit + 3 relay	51507087
30	Power supply 24 VAC/DC non-Ex	Module M3G, power unit + 3 relay	51507089
40	DC/DC convertor for measuring circuit 2	Module M3DC / Ex and non-Ex	51507091
50	Controller module cond. conductive, 2 x current output	Module M3CH-S conductive / Ex + non-Ex	51509506
50	Controller module cond. conductive, 2 x current + HART	Module M3CH-H conductive / Ex + non-Ex	51509507
50	Controller module cond. conductive, PROFIBUS-PA	Module M3CH-PA conductive / Ex + non-Ex	51510992
50	Controller module cond. inductive, 2 x current output	Module M3CH-S inductive / non-Ex	51516046
50	Controller module cond. inductive, 2 x current output	Module M3CH-H inductive / non-Ex	51516043
50	Controller module cond. inductive, PROFIBUS-PA	Module M3CH-PA inductive / Ex + non-Ex	51516048
60	Cond. input module	Module MKIC / Ex + non-Ex	51501206
70	Relay module 3 additional relays	Module M3R-3 / Ex and non-Ex	51507097
70	Relay module 2 Rel. + 1 current input	Module M3R-2 / Ex and non-Ex	51507098
70	Relay module 2 Rel. + 1 resistance input	Module M3R-2 / Ex and non-Ex	51509510
70	Relay module 1 Rel. + 2 current inputs	Module M3R-1 / Ex and non-Ex	51507099
70	Relay module 1 Rel. + 1 current input + 1 resistance input	Module M3R-1 / Ex and non-Ex	51509513
80	Terminal set for cond. input	6-pin terminal + two-pin terminal	xx
90	Jumper set	Five sets of all three jumper types	51507102
100	Partition plate for connection compartment	Five partition plates	51507103
110	Housing upper section non-Ex	Upper section with keypad sheet, connection compartment cover, hinge, des. sign	51507104
120	Housing lower section non-Ex	For one and two-circuit instruments, cpl.	51507106



Note!

For spare part modules for exclusive use in Ex devices, see XA 233C/07/a3.

8.4 Installation and removal of parts

Please observe the danger instructions in chap. 8.3.
The position designations relate to the spare parts list on page 98.

8.4.1 Instrument view

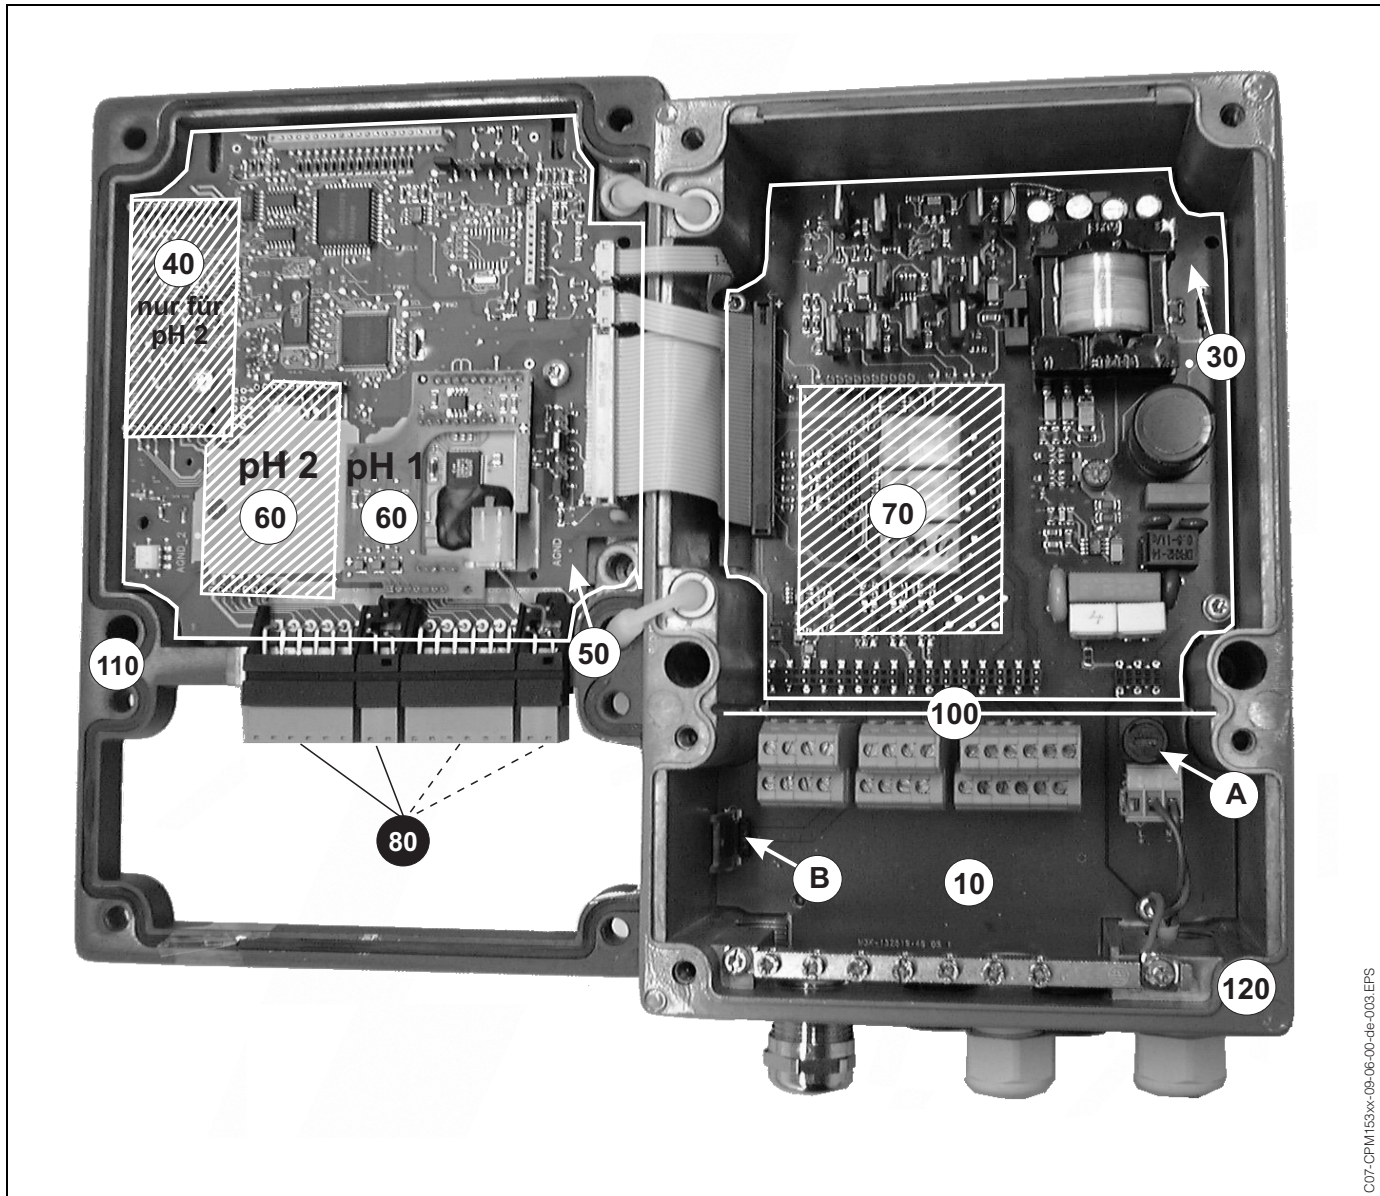


fig. 34: Interior view of the transmitter Mycom S

Remarks:

A: The figure shows the non-Ex fuse.

B: Slot for DAT memory module

40 ... 70: Figure shows module 40. Modules 50, 60 and 70 look somewhat different.

90 ... 120: Figure shows module 90. Modules 100, 110 and 120 look somewhat different.

190: Partition plate (not shown in photo)

80, 130 and dotted position 170: Only available with two-circuit device

C07-CFM153xx-09-06-00-de-003.EPS

8.4.2 Coding

Current outputs active or passive:

For instrument versions CLM153 xxA/Bxx (2 current outputs) and CLM153 xxC/Dxx (2 current outputs with HART) the current outputs can be operated as active or passive. Jumpers on the controller module M3CH allow recoding.

For **non-Ex** instruments, these modules may be recoded to active outputs.



Warning!

Ex instruments must **not** be recoded. Doing so will cause loss of intrinsic safety!

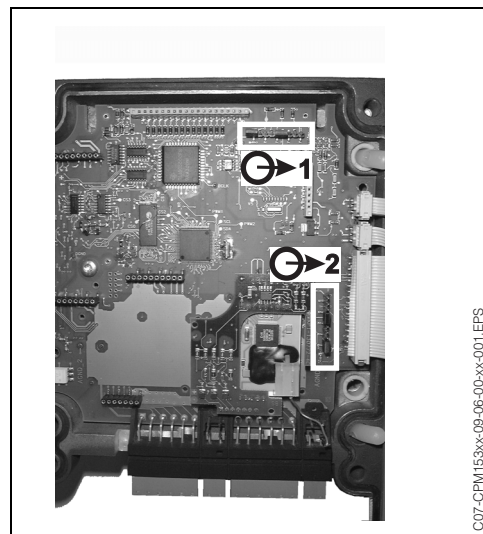


fig. 35: Coding for current outputs
(Interior view of the housing upper section)

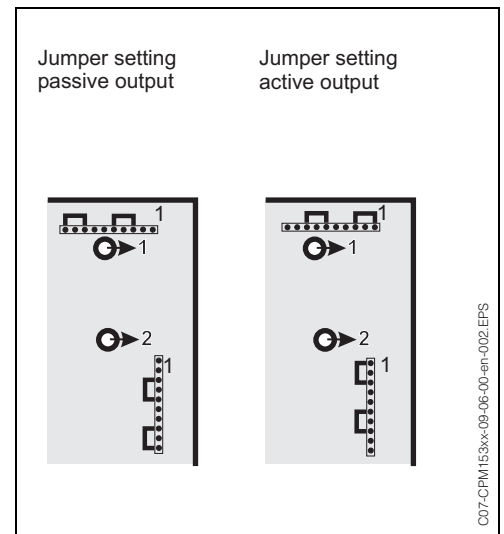


fig. 36: Active/passive coding of the current outputs

8.5 Replacing the device fuses

For non-Ex devices



Warning!

Danger to persons. Before replacing the fuse, make sure the device is voltage-free.

- Position of the fuse holder: "A" in fig. 34
- Use only a 5 x 20 mm fine-wire fuse with 3.15 A, semi time-lag fuse. All other fuses are not permitted.



Caution!

If the fuse should fail again, have the device checked.

8.6 Disposal

The Mycom S CLM153 contains electronic components and PCBs and therefore must be disposed of as electronic refuse. Please keep to the local regulations.

9 Accessories

Offline configuration

The PC tool provides you with a tool for configuring your measuring point at the PC using a simple and self-explanatory menu structure. Write the configuration to the DAT module using the RS232 interface on the PC. The module can then be plugged into the transmitter. You can switch the language via software. The offline configuration system consists of a DAT module, the DAT interface (RS 232) and the software for use with Windows NT/95/98/2000. Order No.: 51507133

DAT module

The DAT module is a memory device (EEPROM) which can be easily plugged into the connection compartment of the transmitter. Using the DAT module you can

- save the complete settings, the logbooks and the data logger of a transmitter and
- copy the complete settings to other CLM153 transmitters with identical hardware functionality.

This considerably reduces the effort to install or service several measuring points. Order No.: 51507175

Assemblies

Type	Properties	Applications
Dipfit W CLA111	Immersion and installation assembly with flange DN 100. The Chemoclean sensor cleaning system can be integrated without any conversion needed. Technical Information: TI 135C/07/en, Order No.: 50076858	■ Water ■ Wastewater ■ Process industry
Dipfit W CYA611	Immersion assembly with thread G 1, G ¾ or NPT ¾". Technical Information: TI 166C/07/en, Order No.: 50085985	■ Water ■ Wastewater
Dipfit P CLA140	Immersion assembly with flange DN 80 PN 16, ANSI 3" 150 lbs or JIS 10K 80A. Sensor holder in bayonet style. Technical Information: TI 1196C/07/en, Order No.: 51500081	■ Wastewater, paper industry

Conductivity sensors

Type	Properties	Applications
Condumax W CLS12/13	Can be adapted to the process for optimum results thanks to different designs. Installation in pipe or flow vessel at temperatures to 250 °C and pressures to 40 bar. Sensor shaft made of die-cast aluminium, sensors of stainless steel 1.4571 (AISI 316 Ti). Technical Information: TI 082C/07/en, Order No.: 50059349	■ Industry ■ Power plants (e.g. condensate measurement) ■ Low conductivities at high pressures and high temperatures
Condumax W CLS15	Sterilisable up to 150°C Polished shaft made of stainless steel 1.4435 (AISI 316L). High accuracy thanks to individually measured cell constant. Installation in pipe or flow vessel. Technical Information: TI 109C/07/en, Order No.: 50065950	■ Monitoring ion exchangers ■ Reverse osmosis ■ WFI (Water for Injection) ■ Chip cleaning
Condumax H CLS16	Pure and ultrapure water sensor: Measuring range from 0.04 to 500 µS/cm. Water-proof connection TOP68 or fixed cable. Hygienic design. Sterilisable up to 150°C EHEDG and 3A certificates. Technical Information: TI 227C/07/en, Order No.: 51503431	■ Pure water ■ Ultrapure water ■ Electro-deionisation ■ Distillation ■ WFI (Water for Injection)
Condumax W CLS21	High chemical, thermal and mechanical stability. Sensor shaft in PES (polyethersulphon). Technical Information: TI 085C/07/en, Order No.: 50059352	■ Monitoring low concentrated saline solutions ■ Potable water treatment ■ Wastewater treatment
Indumax P CLS50	Very chemically stable sensor thanks to PFA jacketing. PEEK version for high temperatures to 180 °C. With  approval. Overall cable length to 55 m. Technical Information: TI 182C/07/en, Order No.: 50090385	■ Chemical industry: ■ Concentration measurement of acids and alkalis ■ Product monitoring ■ Phase separation of product/product mixtures

Type	Properties	Applications
Indumax H CLS52	Sensor shaft made of highly resistant, plastic (PEEK) which can be used with foodstuffs. Very short temperature response times ($t_{90} < 5s$). Measuring range from 10 $\mu S/cm$ to 2000 mS/cm. Technical Information: TI 167C/07/en, Order No.: 50086110	- Foodstuff industry - Control of CIP systems

Service adapter Optoscope

The service adapter aids communication between Endress+Hauser transmitters and the PC using the service interface. You can use it to load new firmware and to save/write customer data (using a PC with the Windows 95/98 or Windows NT operating system).

Chemoclean cleaning

Sensor cleaning can be automated with the injector CYR10 and the appropriate accessories for the different assemblies.

Sensor measuring cable

- Sensor measuring cable CPK9 with TOP68 plug-in head (for high temperature applications, IP 68 / NEMA 6X, also for Ex). Extension with cable CYK71 possible, see table "Measuring cable as yard goods".
- Measuring cable CLK5 for inductive sensors
- Measuring cable CYK71 for conductive sensors
- Junction box VBM: Junction box for extending measuring cable connection between sensor and transmitter. Two threaded joints for e.g. combination sensor.
Material: aluminium casting, ingress protection IP 65. Order No. 50003987

Measuring cables as yard goods

Cable	Description	Order number
CYK71	Measuring cable for conductive conductivity sensors, consisting of a coaxial cable and 4 pilot wires	50085333
	Measuring cable for Ex applications	50085673
CLK5	Extension measuring cable for inductive conductivity sensors CLS50 and CLS52. To be used with the connection box VBM.	50085473

Flat seal


Flat seal for sealing the front panel mounting of the CLM153. Order No.: 50064975

Weather protection cover CYY101

For installing the transmitter outdoors.


Round post fixture for weather protection cover

To fix the weather protection cover to vertical or horizontal posts with diameters of up to 60 mm. Order No.: 50062121

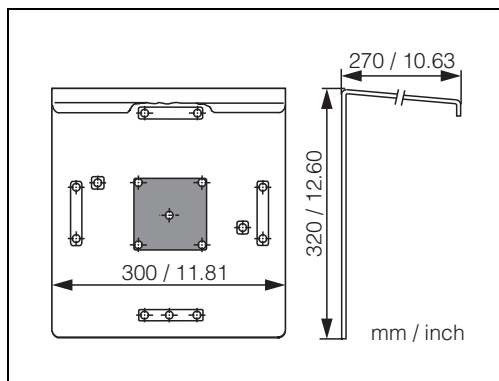

C07-CPM153xx-00-00-en-001.eps

fig. 37: Weather protection cover CYY101

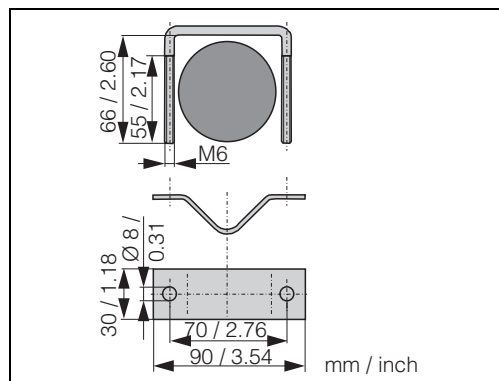

C07-CPM153xx-00-00-en-002.eps

fig. 38: Round post fixture for CYY101

10 Technical data

10.1 Input

Measured variable	Conductivity, resistivity, temperature		
Conductivity, inductive	Measuring range, non-compensated	0.04 $\mu\text{S}/\text{cm}$... 2000 mS/cm	
	Measuring range, compensated	0.04 $\mu\text{S}/\text{cm}$... 1000 mS/cm	
Conductivity, conductive,	Cell constant k	Measuring range	Display range
	0.01 cm^{-1}	0.0 nS/cm ... 600.0 $\mu\text{S}/\text{cm}$	0.0 $\mu\text{S}/\text{cm}$... 200.0 $\mu\text{S}/\text{cm}$
	0.1 cm^{-1}	0.000 $\mu\text{S}/\text{cm}$... 6000 $\mu\text{S}/\text{cm}$	0.000 $\mu\text{S}/\text{cm}$... 2000 $\mu\text{S}/\text{cm}$
	1 cm^{-1}	0.00 $\mu\text{S}/\text{cm}$... 60.00 mS/cm	0.00 $\mu\text{S}/\text{cm}$... 20.00 mS/cm
	10 cm^{-1}	0.0 $\mu\text{S}/\text{cm}$... 600.0 mS/cm	0.0 $\mu\text{S}/\text{cm}$... 200.0 mS/cm
Resistivity measurement	Cell constant k	Measuring range	Display range
	0.01 cm^{-1}	20.0 $\text{k}\Omega\cdot\text{cm}$... 80.0 $\text{M}\Omega\cdot\text{cm}$	20.0 $\text{k}\Omega\cdot\text{cm}$... 37.99 $\text{M}\Omega\cdot\text{cm}$
	0.1 cm^{-1}	2.00 $\text{k}\Omega\cdot\text{cm}$... 2000 $\text{k}\Omega\cdot\text{cm}$	2.00 $\text{k}\Omega\cdot\text{cm}$... 3799 $\text{k}\Omega\cdot\text{cm}$
	1 cm^{-1}	0.200 $\text{k}\Omega\cdot\text{cm}$... 200.0 $\text{k}\Omega\cdot\text{cm}$	0.200 $\text{k}\Omega\cdot\text{cm}$... 379.9 $\text{k}\Omega\cdot\text{cm}$
Concentration measurement	Selection	Conductivity range	Concentration
	NaOH	0.0 mS/cm ... 410 mS/cm	0 ... 15 %
	HNO ₃	0.0 mS/cm ... 781 mS/cm	0 ... 20 %
	H ₂ SO ₄	0.0 mS/cm ... 723 mS/cm	0 ... 20 %
	H ₃ PO ₄	0.0 mS/cm ... 73 mS/cm	0 ... 12 %
	User 1 ... 4	0.0 $\mu\text{S}/\text{cm}$... 2000 mS/cm	0 ... 99.99 %
Temperature	Temperature sensor	Pt 100 (three-wire circuit) Pt 1000 NTC 30k	
	Measuring range (can also be displayed in °F)	−50 ... +150 °C (NTC: −20 ... 100 °C)	
	Measured value resolution	0.1 K	
	Temperature offset	± 5K	
Current inputs 1 / 2 (passive, optional)	Signal range	4 ... 20 mA	
	Input voltage range	6 ... 30 V	

Resistance input (active, optional, only with non-Ex)	Resistance ranges (software switchable)	0 ... 1 k Ω 0 ... 10 k Ω
---	---	---

Binary inputs	Input voltage	10 ... 50 V
	Internal resistance	R _i = 5 k Ω

10.2 Output

Output signal	Conductivity, resistivity, concentration, difference, efficiency, pH, temperature
---------------	---

Signal on alarm	2.4 mA or 22 mA in case of an error
-----------------	-------------------------------------

Load: active current output	max. 600 Ω (non-Ex only)
-----------------------------	---------------------------------

Linearisation / transmission behaviour	Linear, bilinear, table
---	-------------------------

Galvanic isolation	At the same potential are: ■ Current output 1 and power supply ■ Current output 2 and resistance input. The remaining circuits are galvanically isolated from each other.
--------------------	--

Output distribution Current output 0/4...20 mA	Measured error ¹	< 0.2 % of current range maximum
---	-----------------------------	-------------------------------------

Temperature measurement

Output distribution:
17 ... 170 °C

Conductivity measurement

Measuring range:	Output distribution:
0 ... 19.99 μ S/cm	2 ... 19.99 μ S/cm
20 ... 199.9 μ S/cm	20 ... 199.9 μ S/cm
200 ... 1999 μ S/cm	200 ... 1999 μ S/cm
2 ... 19.99 mS/cm	2 ... 19.99 mS/cm
20 ... 2000 mS/cm	20 ... 2000 mS/cm

Resistivity measurement

Measuring range:	Output distribution:
0 ... 199.9 k Ω ·cm	20 ... 199.9 k Ω ·cm
200 ... 1999 k Ω ·cm	200 ... 1999 k Ω ·cm
2 ... 19.99 M Ω ·cm	2.0 ... 19.99 M Ω ·cm
20 ... 200 M Ω ·cm	20 ... 200 M Ω ·cm

Concentration measurement

No minimum spacing

Passive current outputs	Input voltage range	6 ... 30 V
-------------------------	---------------------	------------

Auxiliary voltage output (for binary inputs E1-E3)	Voltage	15 V DC
	Output current	max. 9 mA
Relay contacts	The active open/active closed contact type can be set by software.	
	Switching voltage	max. 250 V AC / 125 V DC
	Switching current	max. 3 A
	Switching power	max. 750 VA
	Lifespan	≥ 5 million switching cycles
Controller output	Function (selectable):	Pulse-length controller (PWM) Pulse-frequency controller (PFM) Three-point step controller (3-PS) Analogue (via current output)
	Switch behaviour	P / PI / PID
	Control gain K_R	0.01 ... 20.00
	Integral action time T_n	0.0 ... 999.9 min
	Derivative action time T_v	0.0 ... 999.9 min
	With the maximum settable frequency in PFM	120 min ⁻¹
	With the maximum settable period length in PWM	1 ... 999.9 s
	With PWM minimum switch-on period	0.4 s
Limit value and alarm functions	Setpoint adjustments	0 ... 100% of display range
	Hysteresis for switching contacts	1 ... 10% of display range
	Alarm delay entry	0 ... 6000 s
Electrical connection	Power supply for CLM153-xxxx 0 xxxx	100 ... 230 V AC +10/-15%
	Frequency	47 ... 64 Hz
	Power supply for CLM153-xxxx 8 xxxx	24 V AC/DC +20/-15%
	Power consumption	max. 10 VA
	Isolation between galvanically isolated circuits	276 V _{rms}
	Terminals, max. cable cross-sectional area	3 x 2.5 mm ²

10.3 Performance characteristics

Measured value resolution	Conductivity: Temperature:	0.001 $\mu\text{S}/\text{cm}$ 0.1 K
Measured error ¹ display	Conductivity, resistivity, concentration: Temperature:	$\pm 0.5\%$ ± 2 digits of measured value < 0.5 K
Measured error ¹ current output	additionally max. 0.2% of current range maximum	
Measured error ¹ current input	max. 1% of measuring range	
Measured error ¹ resistance input	max. 1% of measuring range	
Repeatability ¹	Conductivity, resistivity, concentration: Temperature:	$\pm 0.2\%$ ± 2 digits of measured value max. 0.1% of measuring range

¹: acc. to IEC 746-1, under nominal operating conditions

10.4 Environment

Ambient temperature range	-10 ... +55 °C	
Ambient temperature limits	-20 ... +60 °C	
Storage and transport temperature	-30 ... +80 °C	
Relative humidity	10 ... 95%, non-condensing	
Degree of protection	IP 65	
Electromagnetic compatibility	Interference emission to EN 61326: 1997 / A1:1998; Class B resource (Housing sector) Interference emission to EN 61326: 1997 / A1:1998; Appendix A (Industrial sector)	
Safety requirements	Complies with general safety requirements acc.to EN 61010. Complies with NAMUR Recommendations NE 21,1998.	

10.5 Mechanical construction

Design, dimensions

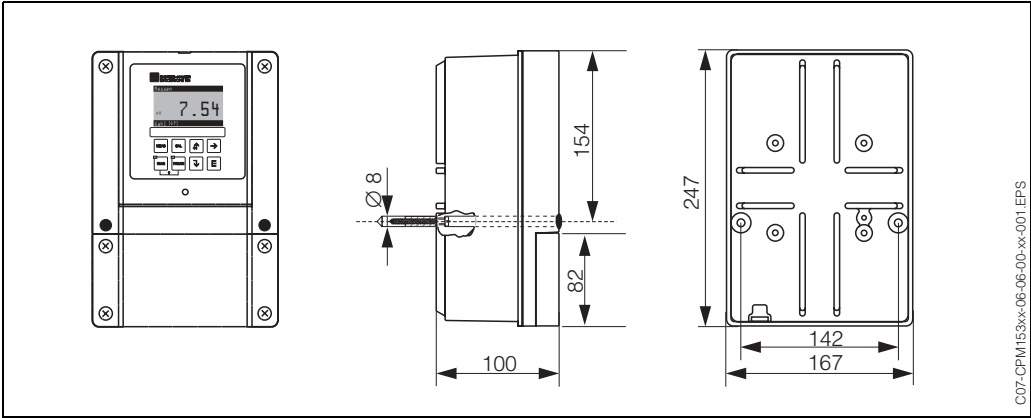



fig. 39: Dimensions of transmitter Mycom S.


Weight	max. 6 kg	
Material	Housing	GD-AlSi 12 (Mg content 0.05%), plastic-coated
	Front	Polyester, UV-resistant


11 Appendix


11.1 Operating matrix


The basic structure of the operating menu is shown below.

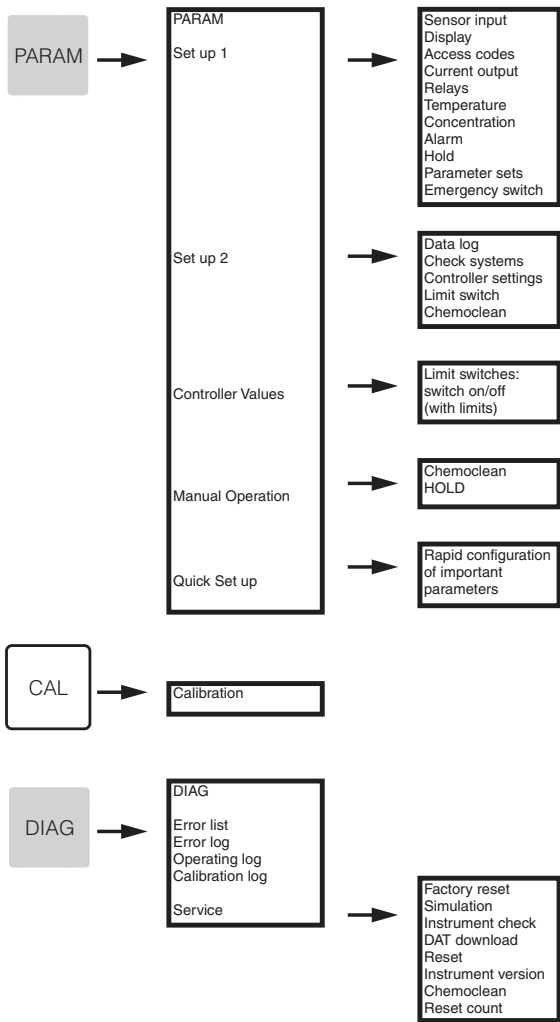

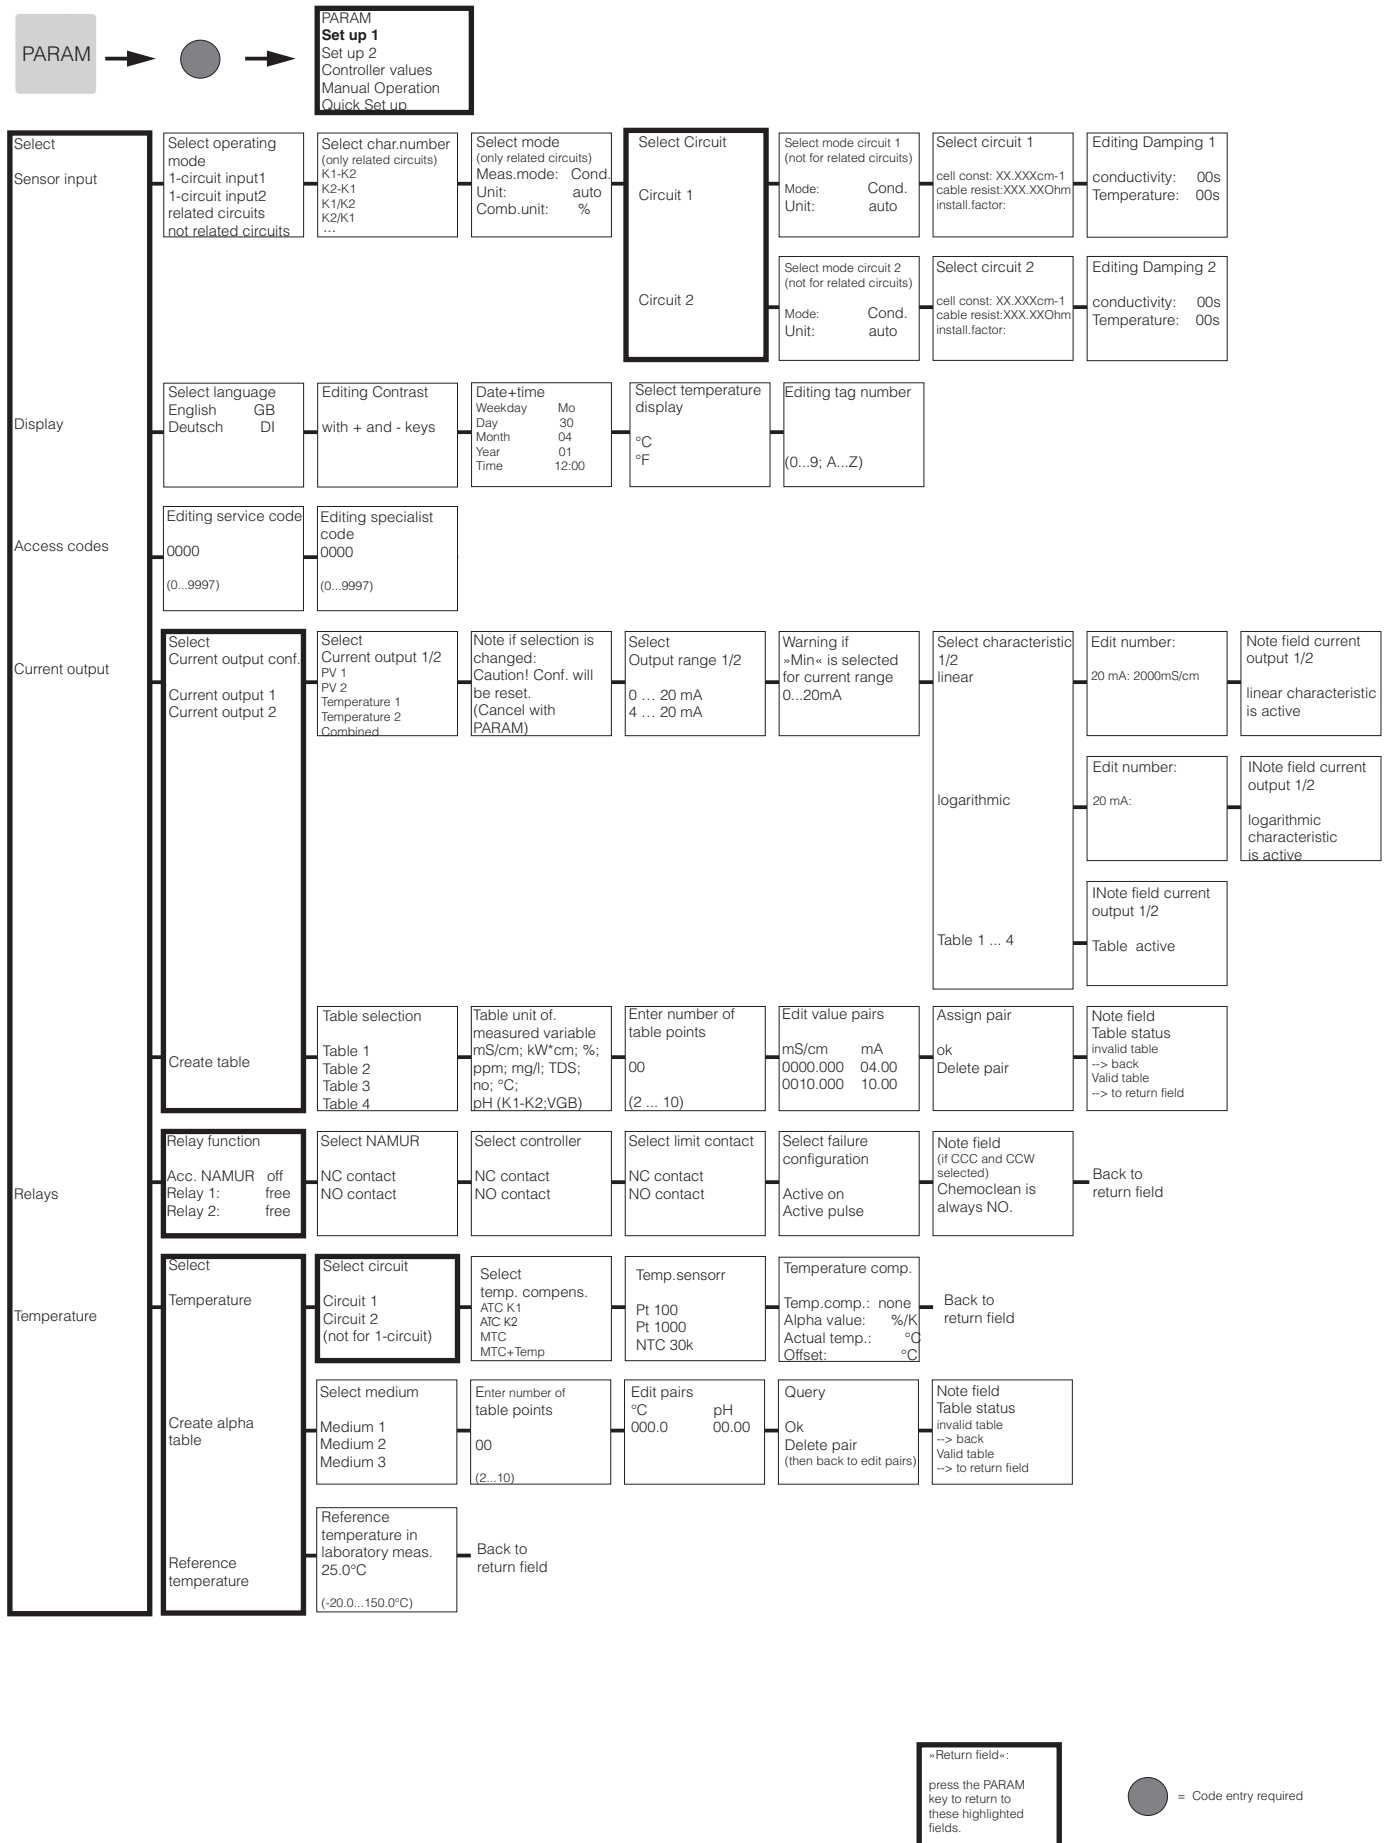

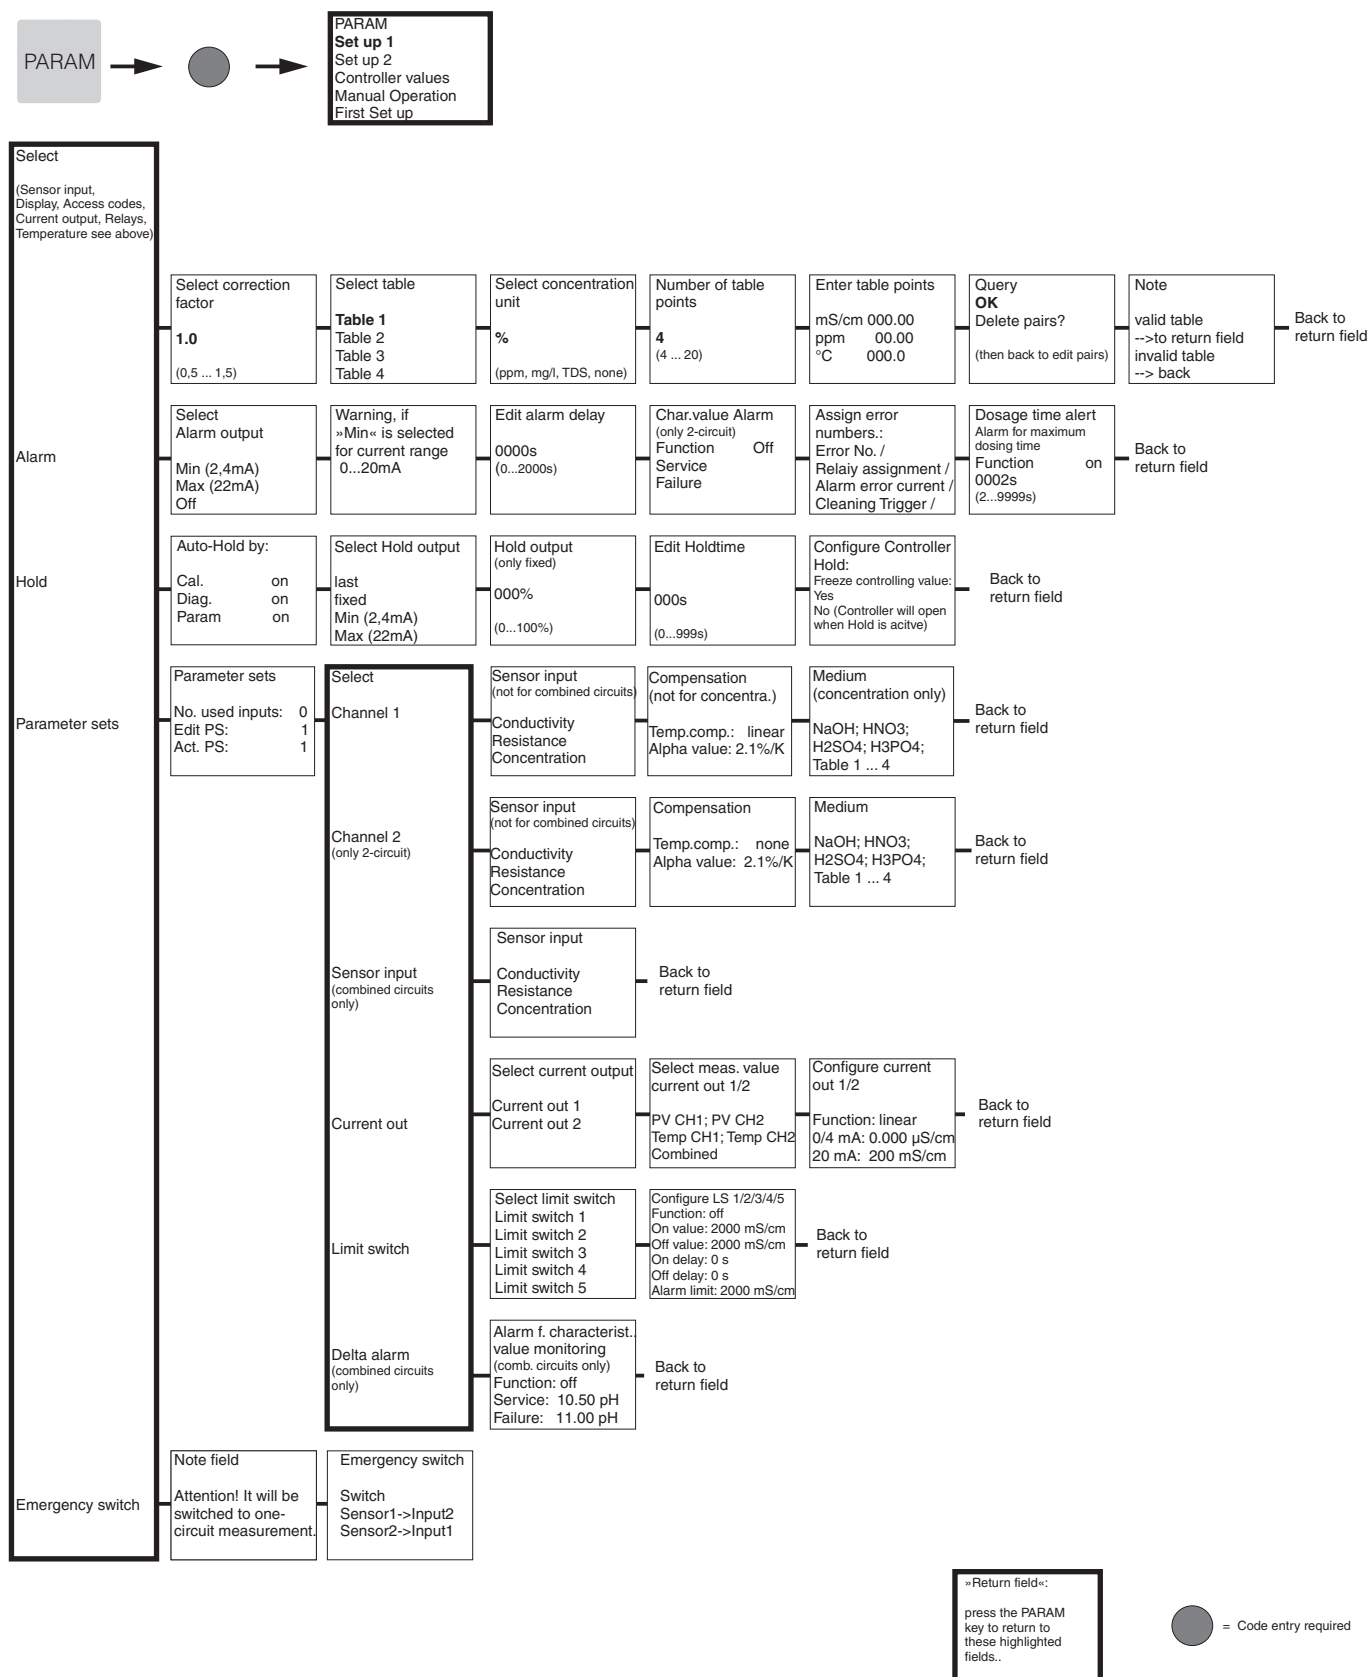


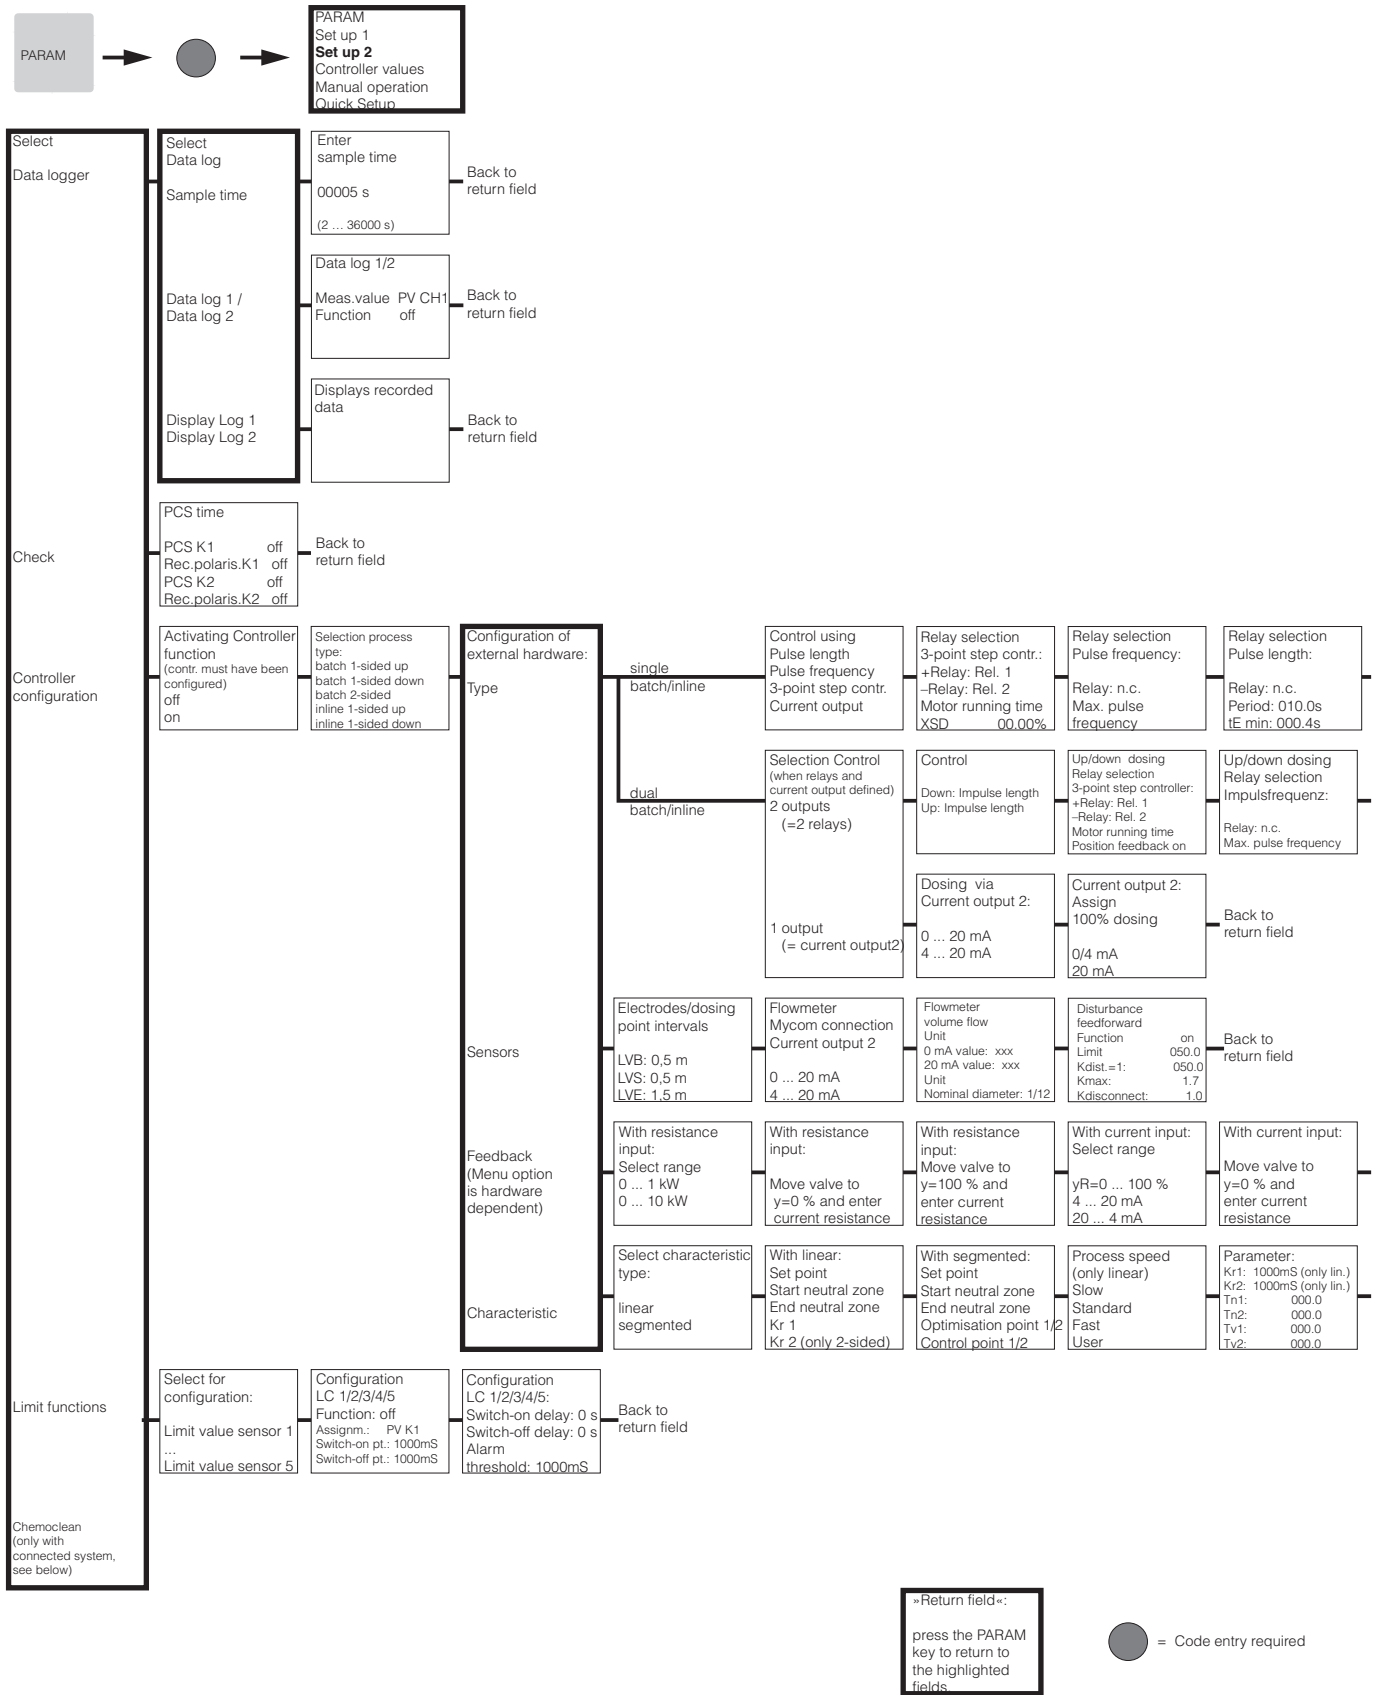

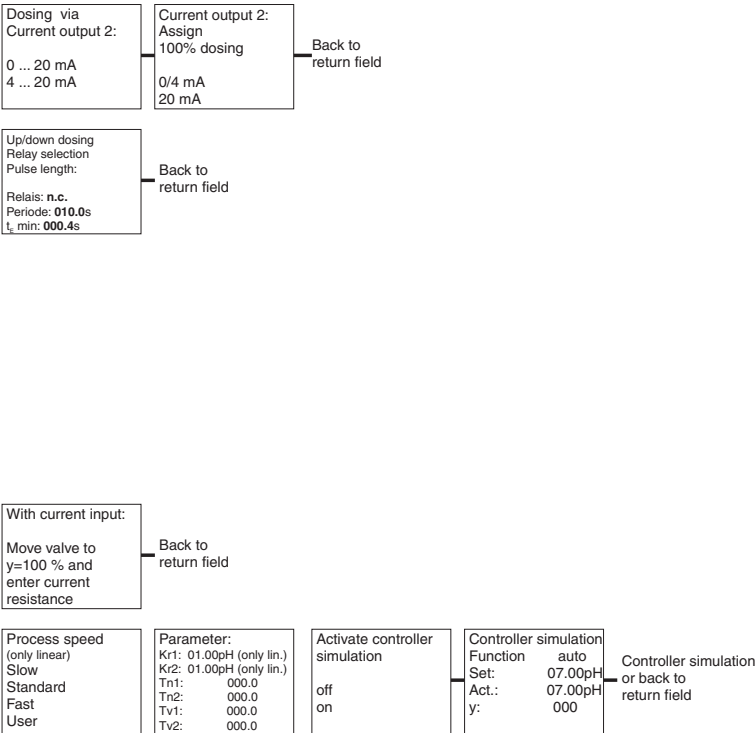


»Return field«:
press the PARAM
key to return to
the highlighted
fields.

 = Code entry required





»Return field«:
press the PARAM
key to return to
the highlighted
fields.

 = Code entry required

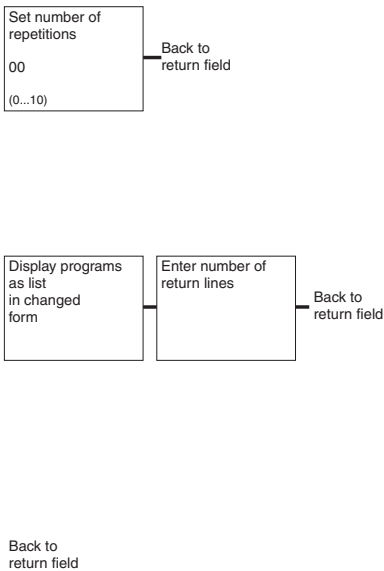


»Return field«:
press the PARAM
key to return to
the highlighted
fields.

 = Code entry required

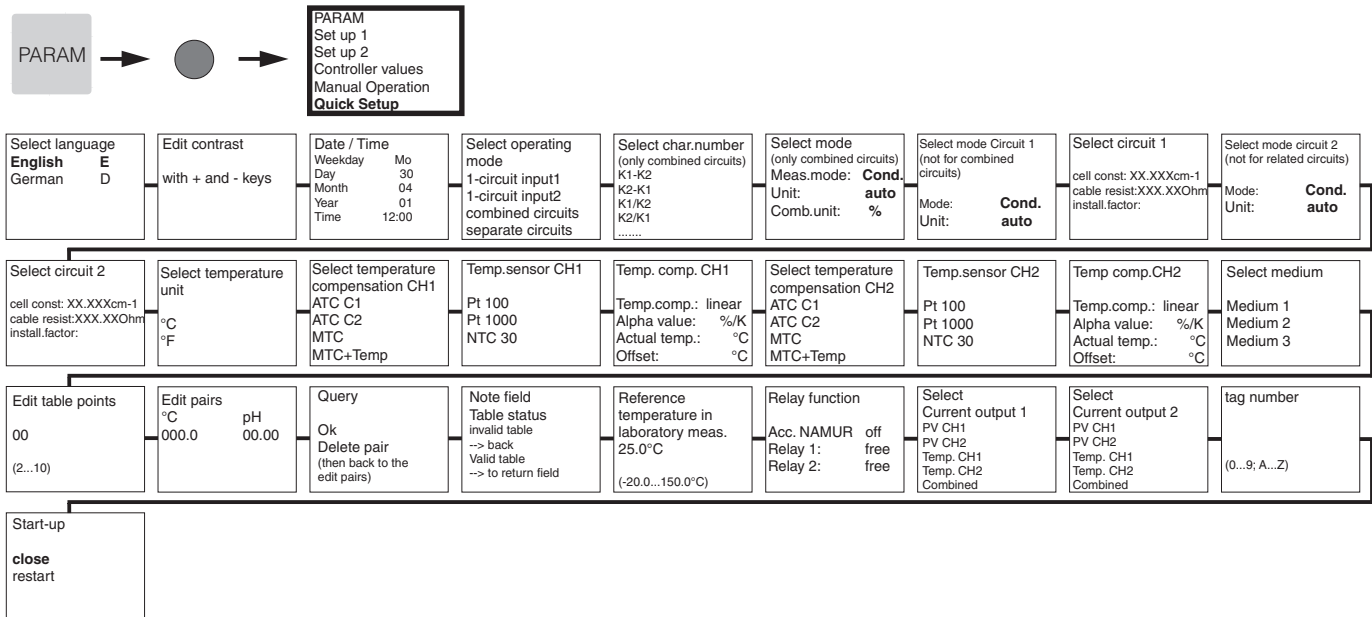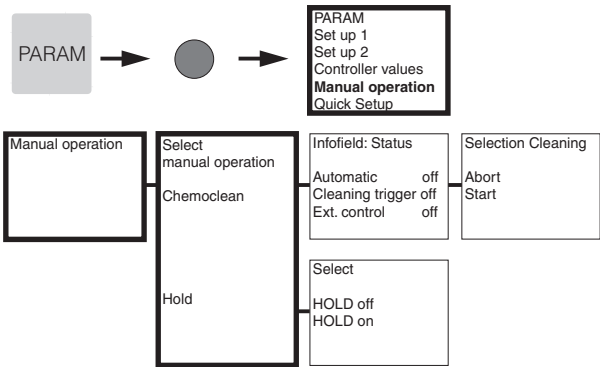


»Return field«:
press the PARAM
key to return to
the highlighted
fields.

[Menu Icon] = Code entry required

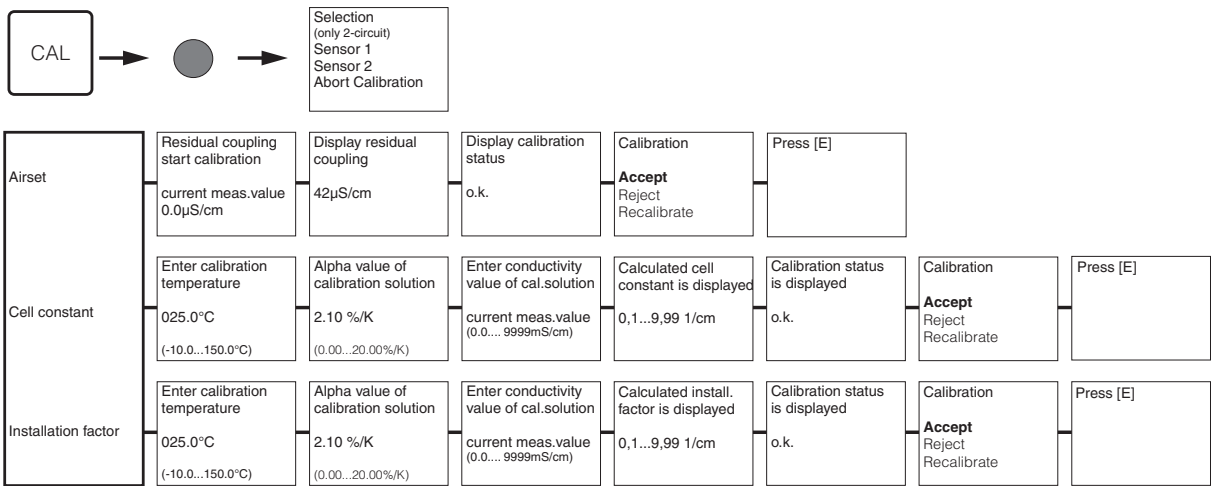

If you press the MEAS key, a message will appear asking if you want to abort the calibration.


 = Code entry required

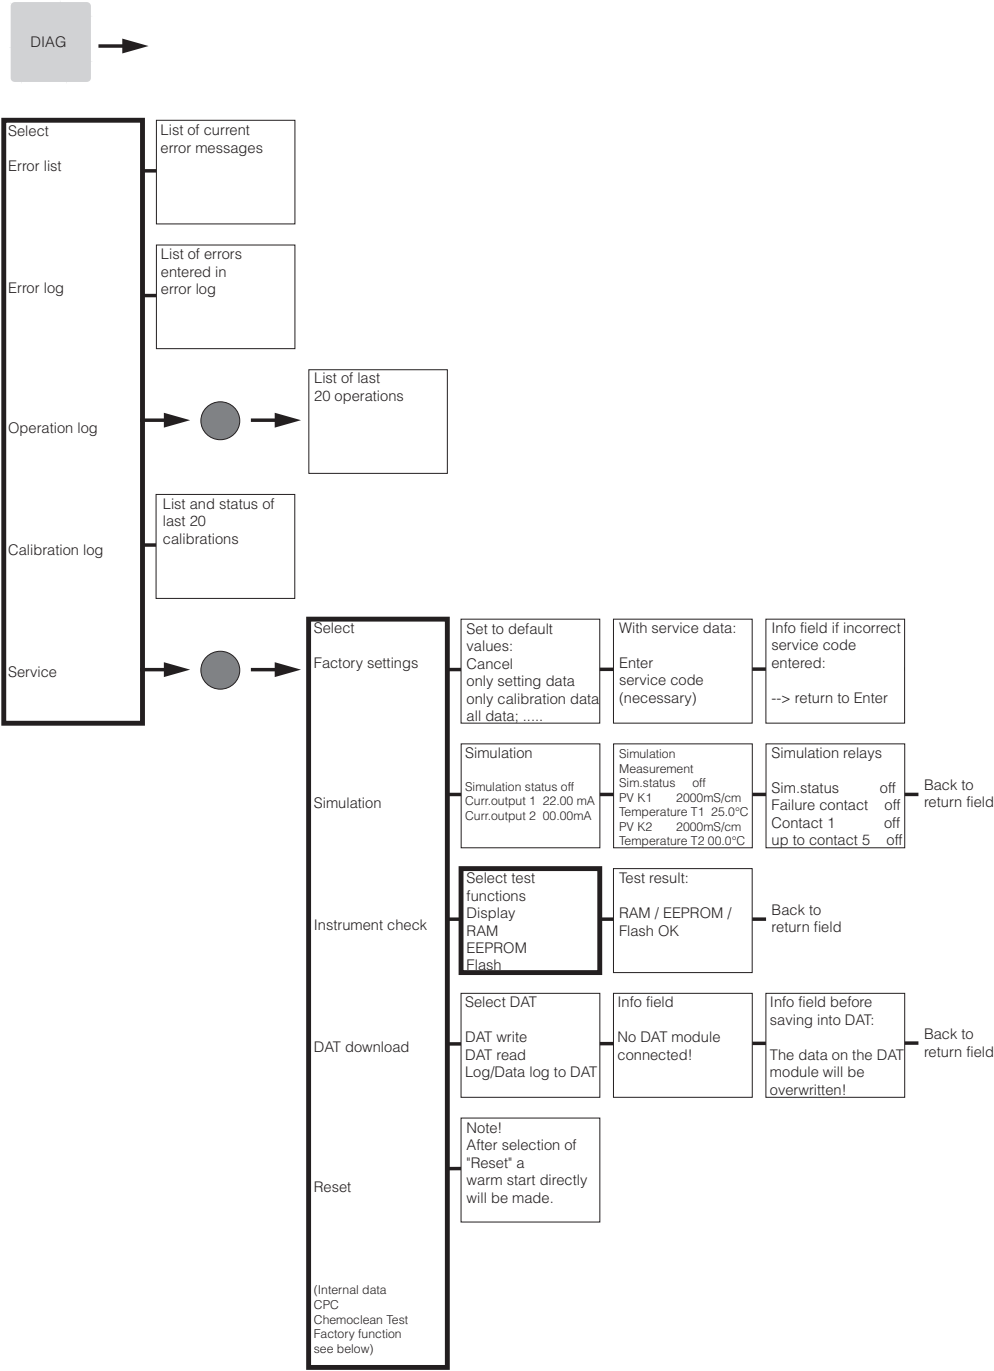

»Return field«:
press the PARAM
key to return to
the highlighted
fields.

● = Code entry required

C07-CLM153xx-19-06-08-en-012.EPS

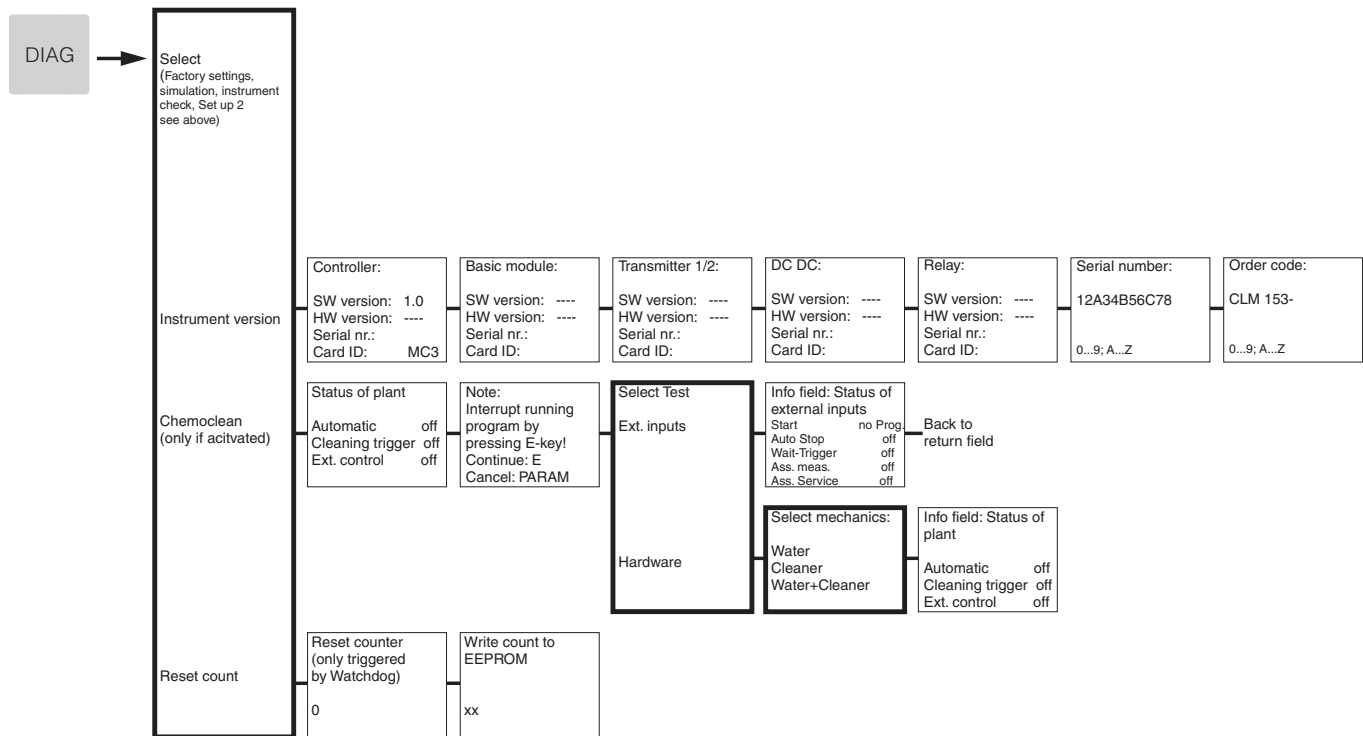

»Return field«:
press the PARAM
key to return to
the highlighted
fields.

 = Code entry required

Index

A

Abnormal transmitter behaviour	81
Access authorisation	21
Accessories	102
Actuator, control	
Analogue	58
Actuators	57, 64
One-sided	64
Two-sided	65
Actuators, control	
Pulse frequency, PFM.	58
Pulse length, PWM.	57
Three-point step controller	58
Adaption factor	27, 85–86
Airset.	85
Alarm	
Delay	49
Dosing time	49
Error current	49
Alarm delay	70
Alarm for characteristic value	49
Alarm menu.	48
Alarm relay	13
Alpha value	42
Formula	44
Ambient temperature	11
Analogue actuator control	58
Appendix.	109
Arrow keys	20
Assemblies.	102
Auxiliary voltage output	13

B

Batch process, pure	57
Binary inputs E1-E3	13
Boards, order numbers	99
Build-up on the sensor	87

C

Cable extension	17
Cable length, maximum	17
Cable resistance	27
Cable types	16
CAL key	20
Calibration	83
Cancelling	83
Protecting (by code)	83
Cancelling calibration	83
Cell constant	84
Certificates and approvals	9
Characteristic	36
Characteristic value	
Alarm	49
Checking	
Conductive sensor	90

Inductive sensor	90
Line extension, boxes	90
ChemoClean	73
Manual operation	74, 78
Chemoclean	73, 103
Cleaning	87
Day programme	75
Weekly programme	75
Cleaning example	74
Cleaning programme	
Edit	76
Cleaning trigger	49
Code	
Activation	21
Maintenance	21
Resetting	21
Specialist	21
Code forgotten?	21
Coding	
Current outputs	101
Combined circuits	26, 32
Commissioning	6, 24
First -	24
Conductivity characteristic	46
Conductivity sensors	102
Configuration	
Enabling	21
Locking	21
Connecting the measuring system	15
Connection compartment label	14
Constant control gain	68
Contact assignment	15, 49
Contact functions	40
Contacts	
Configuring to NAMUR	15
Response to errors	98
Response to power failure	98
Contrast	25, 34
Control gain, range-dependent	68
Control point	68
Control type	64
Controller	
characteristic values	69
Characteristic, constant characteristic	68
Relay assignment	15
Controller characteristic type	68
Controller hold	50
Controller in the CLM 153	61
Controller simulation	69
Controller: Checking the settings	69
Controlling actuators: see Actuators, control	
Current input	68
Current measured values	20

Current outputs	36
Active/passive	101
Controller	64
Dosing up/down	65
Response to errors	98
D	
Damping	33
DAT	
Slot	100
DAT handling	79
DAT module	23, 102
Data logger	
Call up, values	20
Record mode, Scroll mode	21
Date	25, 34
Day programme cleaning	75
Declaration of conformity	9
Delay time, hold	50
Delta alarm	49
Deposits on sensor	87
Descriptions of functions	31
Designated use	6
Determining the characteristic	46
Device designation	8
Device fuse	101
Device reset	79
Device test	
Conductive	88
Inductive	89
DIAG key	19
Diagnosis	79
Digital inputs E1-E3	51
Dimensions	10
Direction of action	57
Disabling programme	77
Display test	80
Displaying calibration log	79
Displaying error list	79
Displaying error log	79
Displaying operation log	79
Disposal	101
Distance electrode – dosing point	66
Dosing time alarm	49
Dosing via current output	65
E	
E key	20
Edit day	75
Edit programme	76
Editor types	22
EEPROM test	80
Electrical connection	106
Electrode contamination	87
Electrode/dosing point distances	66
EMC	7

Enter key	20
Environment	107
Error assignment	49
Error codes	92
Error current	49
Error list	92
Error number list	92
External hold	50

F	
Factory function	79
Factory settings	79
Fault-signalling contact	41
Feedback	67
Feedforward control	67
First commissioning	24
Flash test	80
Flat seal	103
Flow velocity	67
Flowmeter	67
Function check	24

G	
Green LED	20

H	
Help pages	19
Hold	
Controller	50
Current	50
Delay time	50
External	50
On-site	50
Priority	50

I	
Identification	8
Incoming acceptance	10
Inline process, pure	57
Input	104
Installation	6, 10
Installation and removal of parts	100
Installation conditions	10
Installation factor	27, 33, 84–86
Installation instructions	10
Instrument check	79–80
Instrument number	34
Instrument version	79

J	
Junction box VBM	17

K	
Key assignment	19
Keypad test	80
KR	68

L

Language	25, 34
LED	20
Linear characteristic	36
Locking the operation	22
Look-ahead pH measurement	57

M

Mains disconnecting device	14
Maintenance	87
Maintenance code	21
Entry	35
Manual operation	78
ChemoClean	74, 78
Maximum cable length	17
MEAS key	20
Measured value damping	33
Measured value difference monitoring	49
Measured value display	20
Measuring cable	16
Measuring menu for controller	69
Measuring menus	20
Measuring principle	26, 32
Mechanical construction	108
Memory, replaceable (DAT)	23
Menu editor types	22
Modules, order no.	99
Motor run time	58

N

Nameplate	9
NAMUR	15
Class	92
Functions	41
Neutral zone	68

O

Offline configuration	102
One circuit	26, 32
One-sided actuators	64
One-sided process	
Batch	63
Inline	63
On-site hold	50
Operating matrix	109
Operating mode	26–27, 33
Operation	6, 19
Operational safety	7
Optimisation point	68
Optoscope	103
Ordering information	8
Output	105
Output, Technical data	
Output	105

P

Panel mounting	11
----------------------	----

PARAM key	19
Parameter set switching	13, 51
PCS	56
PCS time	56
Performance characteristics	107
PFM	58
Post mounting	11
Post-connection check	18
Post-installation check	12
Power supply	13
Process	57
one-sided	63
two-sided	63
Process check system	56
Product structure	8
Programme	
Enabling	77
Programme cleaning sequence	74
Programme editor	76
PSS	13, 51
Pulse length	64
Pulse-frequency	64
Pulse-frequency controller	58
Pulse-frequency modulation	58
Pulse-length controller	57
Pulse-width modulation	57
PWM	57

Q

Quick Setup	25
Quick wiring guide	13

R

RAM test	80
Range-dependent control gain	68
Red LED	20
Reference temperature	
Temperature compensation	45
Relay	
Configuring to NAMUR	15
Relay assignment	49
Relay contact status	20
Relay selection	64
Renaming programme	77
Replacing the device fuses	101
Reset	79, 81
Codes	21
Counter	82
Data	79
Resistance input	67
Response of contacts to errors	98
Response of contacts to power failure	98
Response of current output to errors	98
Return	7

S

Safety conventions	5
--------------------------	---

Safety icons	5	Output	105
Safety instructions	5	Performance characteristics	107
Scope of delivery	9	Temperature coefficient, alpha	42
Segmented characteristic	68	Temperature sensor	28, 44
Semi-batch process	57	Terminal arrangement	15
Sensor connection	16	Three-point step controller	58, 64
Sensor technology	66	Time	25, 34
Serial numbers	79	Transmitter dimensions	108
Service adapter Optoscope	103	Transport	10
Service data	79	Troubleshooting	91
Service diagnosis	79	Troubleshooting instructions	91
Set up 1	31	Two circuit	26, 32
Set up 2	55	Two-sided actuators	65
Simulation	79	Two-sided process	
Contacts	80	Batch	63
Current outputs	80	Inline	63
Measured value, temperature	80	U	
Simulation f. device test		United States Pharmacopeia	71
Conductive sensors	88	Universal code	21
Inductive sensors	89	Unlocking the operation	22
Slot for DAT memory module	100	User programme	76
Soiling	87	USP	72
Spare parts		USP (United States Pharmacopeia)	71
List	99	W	
Order numbers	98	Wall mounting	11
Specialist code	21	Water for injection	71
Entry of -	35	Weather protection cover CYY 101	12, 103
Storage	10	Weekly cleaning programme	74
Switching on the measuring device	24	Weekly programme cleaning	75
T		WFI	71
Table (characteristic)	36	Wiring	13
Tag number	34	Wiring diagram	13
Technical data	104	Write access	82
Environment	107		
Input	104		
Mechanical construction	108		

Erklärung zur Kontamination

Lieber Kunde,
aufgrund der gesetzlichen Bestimmungen und zum Schutz unserer Mitarbeiter und Betriebseinrichtungen benötigen wir die unterschriebene "Erklärung zur Kontamination", bevor Ihr Auftrag bearbeitet werden kann. Legen Sie diese vollständig ausgefüllte Erklärung unbedingt den Versandpapieren bei. Dies gilt auch für zusätzliche Sicherheitsdatenblätter und/oder spezielle Handhabungsvorschriften.

Geräte- / Sensortyp:	_____	Seriennummer:	_____
Medium / Konzentration:	_____	Temperatur:	_____
Gereinigt mit:	_____	Leitfähigkeit:	_____
		Druck:	_____
		Viskosität:	_____

Warnhinweise zum Medium (zutreffende bitte ankreuzen)



☐
radioaktiv



☐
explosiv



☐
ätzend



☐
giftig



☐
gesundheits-
schädlich



☐
biogefährlich



☐
brandfördernd



☐
unbedenklich

Grund der Einsendung

Angaben zur Firma

Firma:	_____	Ansprechpartner:	_____
	_____		_____
	_____	Abteilung:	_____
Adresse:	_____	Telefon:	_____
	_____	Fax / E-Mail:	_____
		Ihre Auftrags-Nr.:	_____

Hiermit bestätigen wir, dass die zurückgesandten Teile gereinigt wurden und frei sind von jeglichen Gefahren- oder Giftstoffen entsprechend den Gefahrenschutzvorschriften.

(Ort, Datum)

(Firmenstempel und rechtsverbindliche Unterschrift)

For more Endress+Hauser product please visit: www.ainstru.com
Mail: Sales@ainstru.com

www.endress.com/worldwide

BA234C/07/en/04.04
51503794
Printed in Germany / FM+SGML 6.0 /DT



51503794

Endress+Hauser 
People for Process Automation