



Level



Pressure



Flow



Temperature



Liquid
Analysis



Registration



Systems
Components



Services



Solutions

Operating Instructions

Ceramax CPS341D

Sensor with pH-sensitive enamel and
digital Memosens technology

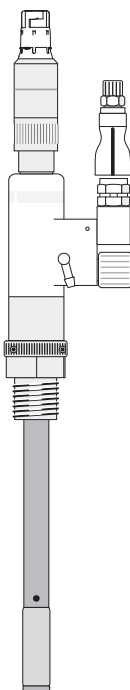


Table of contents

1	Safety instructions	4	9	Technical data	26
1.1	Designated use	4	9.1	Input	26
1.2	Installation, commissioning and operation	4	9.2	Environment	26
1.3	Operational safety	5	9.3	Process	26
1.4	Notes on safety conventions and icons	5	9.4	Mechanical construction	27
2	Identification	6	Index	28	
2.1	Nameplate	6			
2.2	Certificates and approvals	6			
3	Installation	7			
3.1	Overview of sensor	7			
3.2	Installation conditions	8			
3.3	Installing in the process	10			
3.4	Installing the electrolyte vessel	10			
3.5	Mounting the optional electrolyte monitor	11			
4	Wiring	12			
4.1	Connecting the sensor	12			
4.2	Connecting the optional electrolyte monitor	13			
5	Commissioning	14			
5.1	Disinfecting the electrolyte system	14			
5.2	Regenerating the sensor	15			
5.3	Filling the electrolyte vessel	16			
5.4	Calibration	18			
6	Maintenance	19			
6.1	Changing the electrolyte bottle	19			
6.2	Cleaning the sensor	20			
7	Accessories	23			
7.1	CPS341Z	23			
7.2	Transmitter	23			
7.3	Buffer solutions	24			
7.4	Measuring cable	24			
8	Troubleshooting	25			
8.1	Troubleshooting instructions	25			
8.2	Spare parts	25			
8.3	Disposal	25			

1 Safety instructions

1.1 Designated use

The pH sensor is designed for the continuous measurement of the pH value in liquids. Recommended applications include:

- Food production, including thick, high-viscosity media
- Beverage production and filling
- Quality control
- Pharmaceutical industry:
 - Water treatment
 - Active ingredient production
 - Active ingredient preparation
 - Fermentation
 - Biotechnology

Any use other than that described here compromises the safety of persons and the entire measuring system and is, therefore, not permitted.

The manufacturer is not liable for damage resulting from improper or non-designated use.

1.2 Installation, commissioning and operation

Please note the following items:

- Installation, commissioning, operation and maintenance of the measuring system must only be carried out by trained technical personnel.
Trained personnel must be authorized for the specified activities by the system operator.
- Electrical connection must only be carried out by a certified electrician.
- Technical personnel must have read and understood these Operating Instructions and must adhere to them.
- Before commissioning the entire measuring point, check all the connections. Ensure that electrical cables and hose connections are not damaged.
- Do not operate damaged products and secure them against unintentional commissioning. Mark the damaged product as being defective.
- Measuring point faults may only be rectified by authorized and specially trained personnel.
- If faults can not be rectified, the products must be taken out of service and secured against unintentional commissioning.
- Repairs not described in these Operating Instructions may only be carried out at the manufacturer's or by the service organization.

1.3 Operational safety

The sensor is designed to meet state-of-the-art safety requirements, has been tested and left the factory in a condition in which it is safe to operate.

Relevant regulations and European standards have been observed.

As the user, you are responsible for complying with the following safety conditions:

- Installation instructions
- Local standards and regulations

1.4 Notes on safety conventions and icons

The structure, signal words and safety colors of the signs comply with the specifications of ANSI Z535.6 ("Product safety information in product manuals, instructions and other collateral materials").

Safety message structure	Meaning
⚠ DANGER Cause (/consequences) Consequences if safety message is not heeded ► Corrective action	This symbol alerts you to a dangerous situation. Failure to avoid the situation will result in a fatal or serious injury.
⚠ WARNING Cause (/consequences) Consequences if safety message is not heeded ► Corrective action	This symbol alerts you to a dangerous situation. Failure to avoid the situation can result in a fatal or serious injury.
⚠ CAUTION Cause (/consequences) Consequences if safety message is not heeded ► Corrective action	This symbol alerts you to a dangerous situation. Failure to avoid this situation can result in minor or medium injury.
NOTICE Cause/situation Consequences if safety message is not heeded ► Action/note	This symbol alerts you to situations that can result in damage to property and equipment.

2 Identification

2.1 Nameplate

The nameplate can be found on the sensor.

The following information is provided on the nameplate:

- Order code
- Extended order code
- Serial number
- Protection class
- Ambient/process conditions

Compare the data on the nameplate with your order.



To find out what sensor version you have, enter the order code indicated on the nameplate in the search screen at the following address: www.products.endress.com/order-ident

2.2 Certificates and approvals

Declaration of Conformity

The product meets the requirements of the harmonized European standards.

As such, it complies with the legal specifications of the EC directives.



The manufacturer confirms successful testing of the product by affixing to it the **CE** mark.

3 Installation

3.1 Overview of sensor

The CPS341D can be divided into the following parts:

- pH-sensitive part
- Reference system
- Process connection

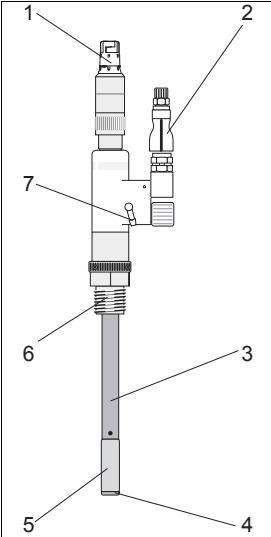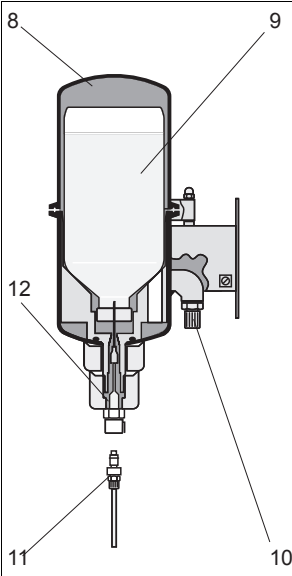pH-sensitive part	Reference system	Process connection
■ Glass-lined steel tube (3) ■ Yellow pH-sensitive enamel with metal reference lead (5) ■ Diaphragm (4) ■ Memosens plug-in head (1)  Fig. 1: 1 Memosens plug-in head 2 Supply of electrolyte 3 Glass-lined steel tube 4 Diaphragm 5 pH-sensitive enamel (yellow) 6 Process connection 7 Vent	■ Electrolyte vessel (8) ■ Electrolyte bottle with septum (9) ■ Supply of electrolyte with hose and plug-in couplings (2 and 11) ■ Reference electrode (in sensor head, not visible from the outside)  Fig. 2: 8 Electrolyte vessel 9 Electrolyte bottle 10 Compressed air connection 11 Electrolyte hose 12 Electrolyte supply coupling	Depends on version ■ M20 ■ Pg 13.5 ■ 3/4" ■ 1" ■ Nozzle DN25 ■ Nozzle DN30 ■ Varivent DN50/40 ■ Sanitary fitting DN50 ■ Sanitary fitting DN25 ■ Tri-Clamp DN50

3.2 Installation conditions

3.2.1 Orientation

The CPS341D can be installed in any position.

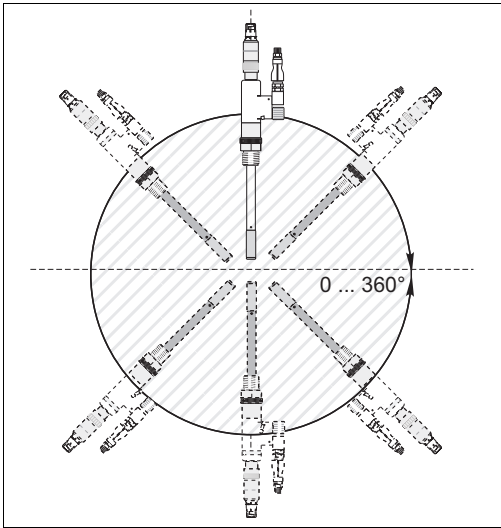


Fig. 3: Installation angle

a0013862

3.2.2 Dimensions

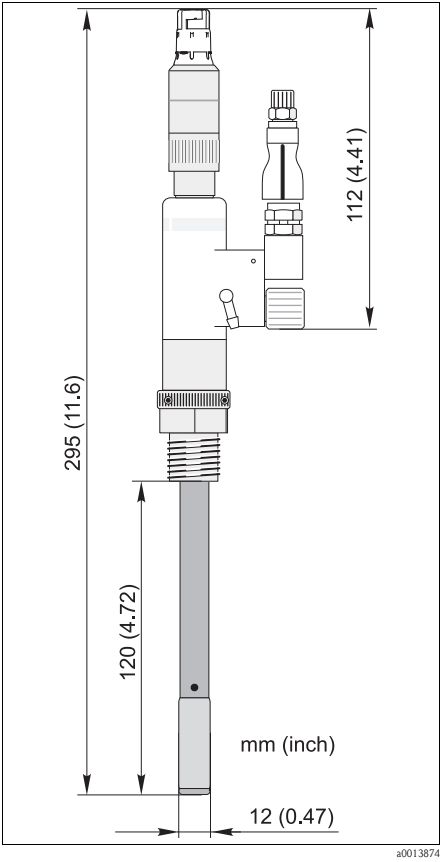


Fig. 4: Dimensions

3.3 Installing in the process

NOTICE

Built-in parts can damage the sensor enamel

► When installing in tanks and pipes, keep a sufficient distance from built-in parts and the wall.

Screw the sensor directly into an existing process connection.

3.4 Installing the electrolyte vessel

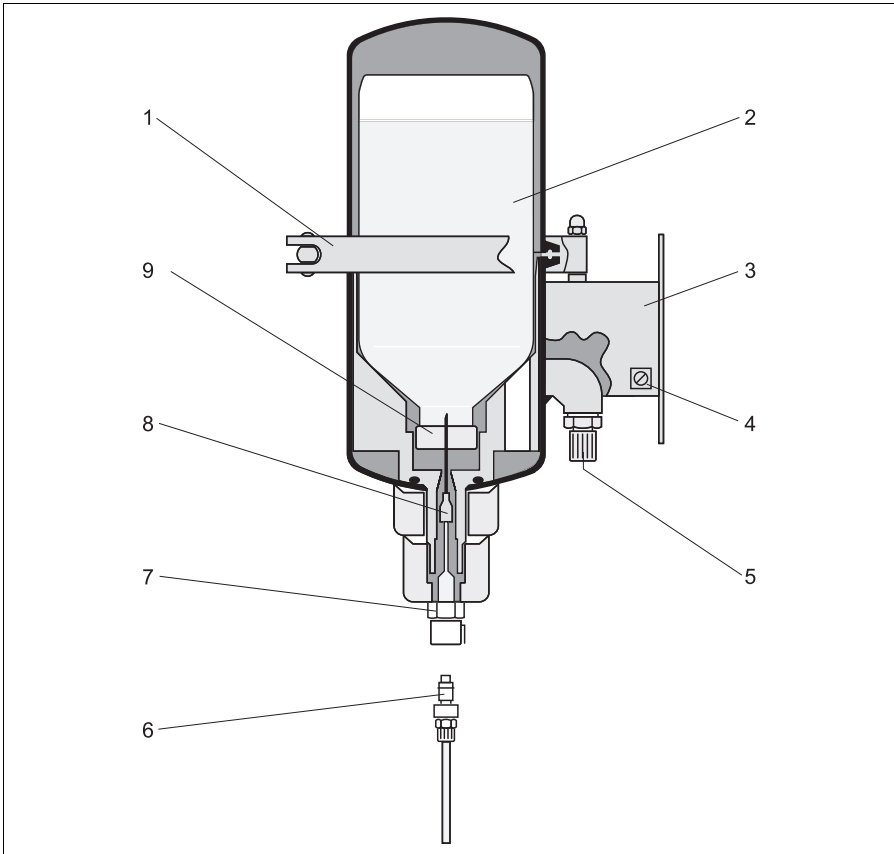


Fig. 5: Electrolyte vessel

a0014009

- | | | | |
|---|--------------------------------|---|--|
| 1 | Clamp | 6 | Self-sealing connector with electrolyte hose |
| 2 | Electrolyte bottle | 7 | Self-sealing coupling |
| 3 | Mounting plate | 8 | Cannula |
| 4 | Ground terminal | 9 | Septum |
| 5 | G1/4 compressed air connection | | |

NOTICE**Minimum internal pressure in electrolyte system**

If the internal pressure is too low, there is the danger of the process medium entering the sensor through the diaphragm and contaminating the electrolyte.

- ▶ Set the compressed air supply in such a way that the pressure in the electrolyte vessel is always at least 0.5 bar (7 psi) above the process pressure.
1. Mount the electrolyte vessel vertically on a wall.
Maximum distance from sensor: 5m (16 ft) (length of the connecting hose).
 2. If necessary, shorten the connecting hose supplied to the desired length.
 3. Connect the hose end with the self-sealing coupling to the connector of the sensor KCl coupling.
 4. Connect the hose end with the self-sealing connector to the coupling of the electrolyte vessel (item 7).
 5. Connect the compressed air supply to the G1/4 gland (item 5) via the onsite pressure-reducing valve.
 6. Set the internal pressure in the electrolyte vessel in such a way that the pressure is at least 0.5 bar above the process pressure but does not exceed the permitted sensor process pressure of 6 bar (90 psi).



A higher difference in pressure is possible but increases the rate of electrolyte consumption.

3.5 Mounting the optional electrolyte monitor

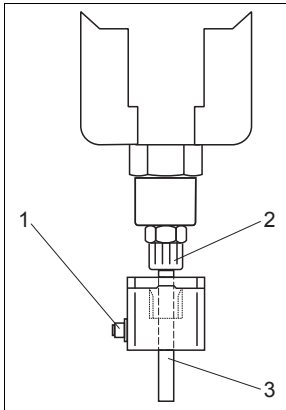


Fig. 6: Electrolyte monitor

a0014091

1. Unscrew the cover of the electrolyte monitor (bubble sensor).
2. Fit the bubble sensor at the outlet of the electrolyte vessel (2) onto the hose (3).
3. Screw the cover back on.
4. Connect the plug of the connecting cable CPS341Z-D3 to the M12 connection (1).



Always order the connecting cable with the bubble sensor as the sensor cannot work without the cable.
For information on how to connect the external supply voltage,
→ see the "Wiring" section

4 Wiring

4.1 Connecting the sensor

The sensor is electrically connected to the transmitter via the special measuring cable CYK10.

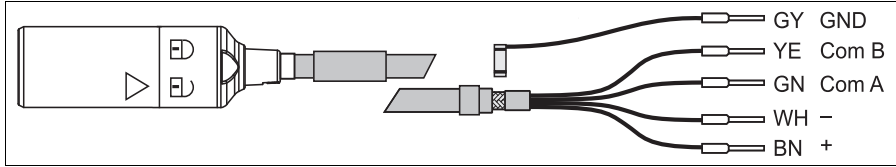


Fig. 7: Special measuring cable CYK10

a0003350

NOTICE

Zero point shift

If the sensor is immersed in medium and the transmitter is disconnected from the power supply, polarization can cause an **irreversible** zero point shift. In such instances, the device must be recalibrated.

- ▶ Do not disconnect the transmitter from the power supply while the sensor is immersed in the medium.
- ▶ When performing maintenance work or similar with the sensor connected, remove the sensor from the medium and dry it before disconnecting the transmitter from the power supply.
- ▶ In general, avoid any kind of conductive connection between the reference and the pH-sensitive enamel when the unit is switched off.
- ▶ If you have taken the sensor out of the medium, it is **essential** you use the KCl protection cap specially designed for CPS341D to protect the diaphragm.

4.2 Connecting the optional electrolyte monitor

1. Connect the connecting cable to an **onsite power supply provided by the customer** (see examples).
2. Connect the M12 plug to the M12 connection of the bubble sensor (if not already performed during installation).

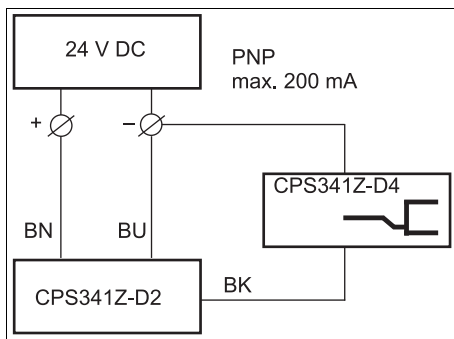


Fig. 8: Connecting to the customer power supply with a relay

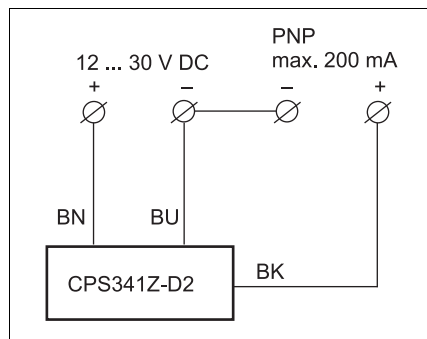


Fig. 9: Connecting to the customer power supply with a PLC

- i** Light emitting diodes in the cable connector indicate the status in the electrolyte supply system:
- Green = supply voltage on
 - Green + yellow = air bubble in the hose (electrolyte vessel empty)

5 Commissioning

Prior to initial commissioning, make sure that:

- The sensor has been installed correctly
- The electrical connection is correct

Several steps are involved in the process of commissioning the sensor:


1. Disinfecting the electrolyte system (optional, for sterile applications)
2. Regenerating the sensor
3. Filling the electrolyte vessel
4. Calibrating/adjusting the sensor

5.1 Disinfecting the electrolyte system

For sterile applications, you can disinfect the entire electrolyte system with 70% ethanol **prior to commissioning** (ethanol is not included in the scope of supply).


 The sensor parts in contact with the medium must be sterilized by appropriate means (SIP).

1. Insert the ethanol bottle

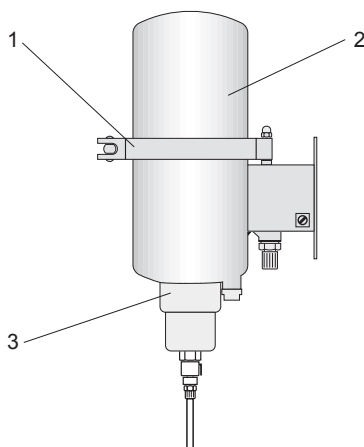

- a. Release the clamp (1) on the mounted electrolyte vessel and remove the upper part (2).
- b. Fill an empty septum bottle (see "Accessories") with 70% ethanol.
- c. Place the bottle into the bottom part of the electrolyte vessel with the septum in a central position and pointing downwards. This causes the cannula of the electrolyte vessel to pierce the septum.
- d. Fit the upper part and seal the device tightly with the clamp.
- e. If you have not already done so, connect the electrolyte vessel and the sensor via the electrolyte hose that can be plugged in at both ends.

2. Disinfect the electrolyte system

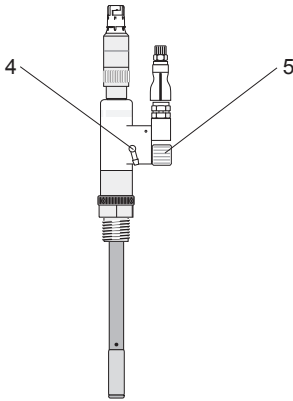

- a. Apply at least 3 bar (45 psi) pressure to the electrolyte vessel.
 - b. Open the vent screw on the sensor (5) (one revolution) until approx. 50 to 100 ml of ethanol flows out of the vent opening (4).
 - c. Allow the ethanol to take effect for 2 to 5 minutes.
3. Remove the ethanol bottle
 - a. Switch off the compressed air and release the pressure on the electrolyte vessel (release the thread adapter nut on the plastic insert (Fig. under 1., item 3) by 2-3 revolutions).
 - b. Once the vessel is unpressurized tighten the thread adapter nut immediately.
 - c. Release the clamp on the electrolyte vessel and remove the upper part.
 - d. Remove the ethanol bottle.
 4. Fill the sensor with electrolyte (→ following section) directly after disinfecting the unit.

5.2 Regenerating the sensor

Slightly larger measured errors can occur during commissioning when using new sensors and sensors that have been dry for extended periods. Regeneration eliminates these measured errors. During the regeneration process, the necessary gel layer is formed on the surface of the pH-sensitive enamel.

 If the sensor is cleaned and sterilized in the tank or pipe before commissioning, additional regeneration is not required.

The sensor is regenerated with the sensor installed and connected. The transmitter must be switched on.

There are three possible ways to regenerate the sensor:


1. Wet the sensor for 12-24 hours.
2. Immerse the sensor in hot water (temperature of 70 to 100 °C (160 to 210 °F)) for approximately 30 minutes.
3. Treat the sensor with water vapor for 10 to 15 minutes.

5.3 Filling the electrolyte vessel

The electrolyte must be free from bubbles. This is the only way to ensure the correct electrical connection between the reference electrode and the diaphragm.


i The electrolyte is 3M KCl (pH 4) with an added inhibitor (1 ml/l colloidal silicic acid) which prevents the formation of bacteria.

1. Insert the electrolyte bottle (see "Accessories")

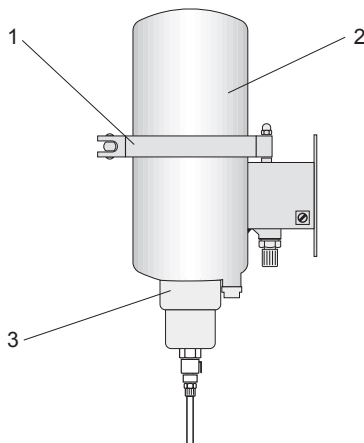

- a. Release the clamp (1) on the electrolyte vessel and remove the upper part (2).
- b. Remove the read seal cap on the bottle of electrolyte.
- c. Place the bottle into the bottom part of the electrolyte vessel with the septum in a central position and pointing downwards. This causes the cannula of the electrolyte vessel to pierce the septum.
- d. Fit the upper part and seal the device tightly with the clamp.

2. Fill the electrolyte system

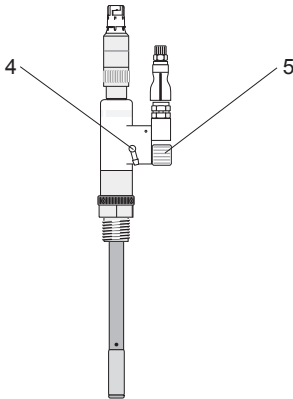

- a. Apply at least 3 bar (45 psi) pressure to the electrolyte vessel.
- b. If you have not already done so:
 - Connect the electrolyte vessel and the sensor via the electrolyte hose that can be plugged in at both ends.
 - Connect the sensor to the transmitter and switch on the transmitter.
- c. Open the vent screw on the sensor (5) (one revolution) until bubble-free electrolyte exits the vent opening (4).
 -  If you disinfected the electrolyte system beforehand, allow at least 50-100 ml of electrolyte to escape.
- d. Close the vent screw and clean the sensor around the vent opening with water.
- e. Establish the process pressure in the electrolyte vessel.

5.4 Calibration

5.4.1 Need for calibration

The calibration data are stored in the Memosens head at the factory and are transferred to the transmitter.

The sensor is ready to measure immediately.

It is recommended to verify the calibration data and recalibrate if necessary if the device has not been in operation for an extended period.

Perform the calibration as specified in the Operating Instructions of the transmitter.

5.4.2 Types of calibration

The following types of calibration are possible:

- Two-point calibration
 - With calibration buffers
 - Entry of data for the slope, zero point and temperature
- Single-point calibration
 - Entry of an offset or a reference value
 - Sample calibration with laboratory comparative value
- Temperature adjustment by entering a reference value

6 Maintenance

6.1 Changing the electrolyte bottle


- i** You should change the bottle before it is completely empty. In this way, you can ensure that the electrolyte system is always full.
- If you are using the optional electrolyte monitor, a message is activated when the first air bubble is detected at the outlet of the vessel. Then replace the bottle of electrolyte within the next 10 hours.

NOTICE

Process pressure and process temperature


Medium penetrating the system can contaminate the sensor reference system

- ▶ Only replace the bottle of electrolyte when no process pressure is applied and at temperatures below 80 °C (176 °F).
 - ▶ If this is not possible, you must replace the bottle very quickly.
1. Disconnect the electrolyte hose from the outlet of the electrolyte vessel by pressing the unlocking unit on the coupling (4) and removing the hose with the connector. The pressure is maintained briefly in the hose and sensor.

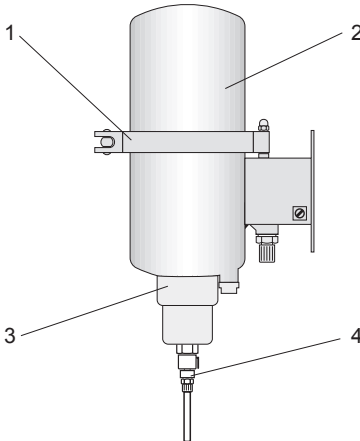

2. Switch off the compressed air and release the pressure on the electrolyte vessel (release the thread adapter nut on the plastic insert (item 3) by 2-3 revolutions).
3. Insert the electrolyte bottle
 - a. Release the clamp (1) on the electrolyte vessel and remove the upper part (2).
 - b. Place the bottle of electrolyte into the bottom part of the electrolyte vessel with the septum in a central position and pointing downwards. This causes the cannula of the electrolyte vessel to pierce the septum.
 - c. Fit the upper part and seal the device tightly with the clamp.

4. Reinsert the (self-sealing) connector of the electrolyte hose into the coupling on the electrolyte vessel.
5. Fill the electrolyte system

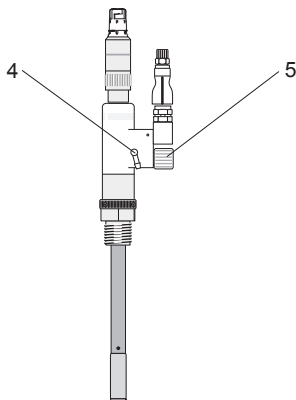

- a. Apply at least 3 bar (45 psi) pressure to the electrolyte vessel.
- b. Open the vent screw on the sensor (5) (one revolution) until bubble-free electrolyte exits the vent opening (4).
- c. Close the vent screw and clean the sensor around the vent opening with water.
- d. Establish the process pressure in the electrolyte vessel.

6.2 Cleaning the sensor

6.2.1 Cleaning agent

Suitable cleaning agents

- Water or solvents
- Non-scratch stainless steel cleaner
- Diluted hydrochloric acid (5 to 20%)

NOTICE

Fluorinated acids and abrasive cleaners

Fluorinated acids (e.g. hydrofluoric acid) and abrasive substances corrode the enamel.

- ▶ Never use fluorinated acids to clean the sensor.
- ▶ Do not use metal or abrasive cleaning agents.

6.2.2 Cleaning the sensor

NOTICE

Acids and alkalis

If the permitted process limits are exceeded, this can increase the level of enamel corrosion

- ▶ Avoid exceeding the maximum permitted values for temperatures and cleaning times.
- ▶ Please note that when cleaning with alkalis, the level of corrosion doubles with every 10 °C increase in temperature.
- ▶ Do not use acid or alkali concentrations that are higher than the permitted concentration levels.

The sensor can be cleaned in place (CIP).

■ Example:

1. 2% alkali, 85 °C (176 °F), 1 hour
2. 1.5% acid, 60 °C (140 °F), 15 minutes
3. Water vapor, 135 °C (275 °F)

- Cleaning with alkaline media affects the gel layer of the enamel. This results in a zero point shift which, in turn, causes temporary measured errors.
- Regenerating the sensor by treating it subsequently with steam regenerates the gel layer and rectifies the zero point shift.

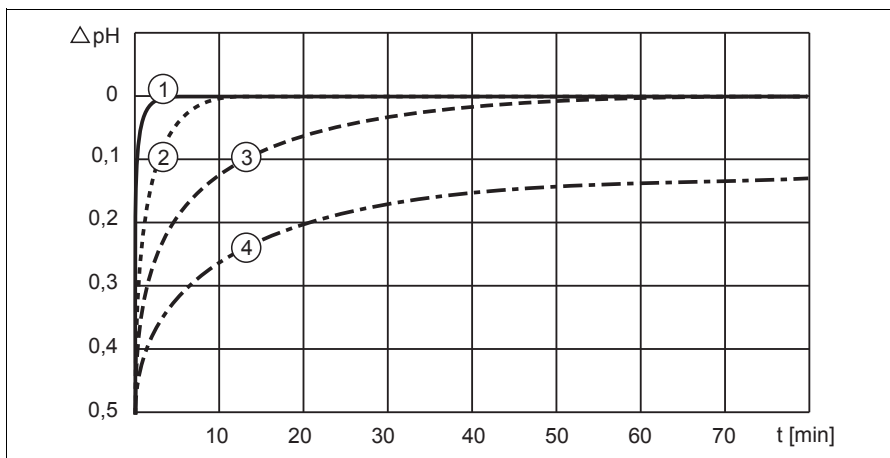


Fig. 10: Regeneration after 30-minute CIP with 2%NaOH at 85 °C (185 °F)

- 1 Regeneration with steam, 135 °C (275 °F)
- 2 Regeneration with water, 95 °C (203 °F)
- 3 Regeneration with water, 80 °C (176 °F)
- 4 Regeneration with water, 25 °C (77 °F)

a0014075

6.2.3 Sterilizing the sensor

The sensor can be sterilized in place (SIP). The following are permitted for SIP:

- Process medium
- Water vapor
- Alcohol solutions
- Aseptic solutions

7 Accessories

-  The most important accessories available at the time this document went to print are listed below.
Please contact your sales center or service organization for accessories that are not listed here.

7.1 CPS341Z

-  Correct function of Ceramax CPS341D depends on reliable supply of KCl to the reference part of the sensor. The pressurized electrolyte vessel CPS341Z-D1 is best suited for this.

The electrolyte supply can be monitored by the ultrasonic sensor for level monitoring CPS341Z-D2 (air bubble sensor). The ultrasonic sensor requires a supply voltage of 18 to 30 V DC at a max. of 70 mA (without switching current).
The signal is output via the relay CPS341Z-D4 as well as optically via the LED display CPS341Z-D3.

	Accessories for Ceramax CPS341D
A1	Welding nozzle DN30, straight
A2	Dummy plug for welding nozzle DN30
A3	Welding nozzle DN25, straight
A4	Welding nozzle DN25, inclined
D1	Electrolyte vessel, stainless steel
D2	Ultrasonic sensor level monitoring
D3	Cable with LED display
D4	Relay, type KCD2-R, P+F
D5	KCl electrolyte, sterile, 1 l plastic bottle
D6	Purified water, sterile, 1 l plastic bottle
D7	Plastic bottle, empty
D8	Protection cap
CPS341Z-	

To obtain a valid order code, simply append the optional features to the order code. If you have any questions, please contact our sales office.

7.2 Transmitter

- Liquiline CM44x
- Multichannel transmitter for connecting digital sensors with Memosens technology
 - Power supply 85 to 265 V AC, 18 to 36 V DC or 20 to 28 V AC
 - Universally upgradeable
 - SD card slot
 - Alarm relay
 - IP 66, IP 67, NEMA 4X
 - Order as per product structure (Technical Information TI444C/07/en)

Liquiline M CM42

- Modular two-wire transmitter for hazardous and non-hazardous areas
- Hart®, PROFIBUS or FOUNDATION Fieldbus available
- Order as per product structure, Technical Information TI381C/07/en

Mycom S CPM153

- Transmitter for pH and ORP
- Ex or non-Ex
- Hart® or PROFIBUS possible
- Order as per product structure, Technical Information TI233C/07/en

 Liquisys CPM223/253 is not recommended. The CPM223/253 software does not fully support the function of Ceramax CPS341D.

7.3 Buffer solutions

High-quality buffer solutions of Endress+Hauser - CPY20

The secondary buffer solutions have been referenced to primary reference material of the PTB (German Federal Physico-technical Institute) and to standard reference material of NIST (National Institute of Standards and Technology) according to DIN 19266 by a DKD (German Calibration Service) accredited laboratory.

		pH value	
	A	pH 2.00 (accuracy ± 0.02 pH)	
	C	pH 4.00 (accuracy ± 0.02 pH)	
	E	pH 7.00 (accuracy ± 0.02 pH)	
	G	pH 9.00 (accuracy ± 0.02 pH)	
	I	pH 9.20 (accuracy ± 0.02 pH)	
	K	pH 10.00 (accuracy ± 0.05 pH)	
	M	pH 12.00 (accuracy ± 0.05 pH)	
		Quantity	
	01	20 x 18 ml (0.68 fl.oz) only buffer solutions pH 4.00 and 7.00	
	02	250 ml (8.45 fl.oz)	
	10	1000 ml (0.26 US gal)	
	50	5000 ml (1.32 US gal) canister for Topcal S	
		Certificates	
	A	Buffer analysis certificate	
		Version	
	1	Standard	
CPY20-		complete order code	

7.4 Measuring cable

Memosens data cable CYK10

- For digital sensors with Memosens technology:
pH, ORP, oxygen (amperometric), chlorine, conductivity (conductive)
- Order as per product structure, see Technical Information (TI376C/07/en)

8 Troubleshooting

8.1 Troubleshooting instructions

Problem	Cause	Remedial action
Value displayed fluctuates when the electrolyte hose is touched	■ Not vented sufficiently ■ Overpressure too low	■ Vent ■ Check and increase pressure
Reading does not change in media with different pH values	Pinhole in pH enamel/insulation error	Have repaired by the Service Team
Zero point drifts, is no longer in permitted range and shifts during venting	Reference electrode defective	Have repaired by the Service Team
Slope too low or very slow reaction	Limescale or other material buildup	■ Measure potential at pH 3 and pH 7 ■ Check slope, $\rightarrow$ min. 55 mV/pH at 25 °C ■ Immerse sensor in 10% HCl for 30 minutes, then wet and measure again ■ If acid treatment does not have the desired effect: Have the unit checked by the Service Team

8.2 Spare parts

Order number	Name
71118068	CPS341D kit, O-ring set for DN25
71118070	CPS341D kit, O-ring set for DN30
71118071	CPS341D kit, O-ring set for diff. types
71118072	CPS341D kit, clamp seal, DIN DN100
71118073	CPS341D kit, complete pressure vessel insert
71118074	CPS341D kit, complete cannula holder
71118075	CPS341D kit, electrolyte vessel connection

8.3 Disposal

The device contains electronic components and must therefore be disposed of in accordance with regulations on the disposal of electronic waste.

Observe local regulations.

9 Technical data

9.1 Input

9.1.1 Measured variables

pH value

Temperature

9.1.2 Measuring range

0 to 10 pH (linear range)

-2 to 14 pH (operating range)

0 to 140 °C (32 to 280 °F)

9.2 Environment

9.2.1 Ambient temperature range

The sensor may not be used at temperatures below 0 °C (32 °F).

9.2.2 Storage temperature

0 to 50 °C (32 to 120 °F)

9.2.3 Degree of protection

IP 68 (10 m (33 ft) water column, 25 °C (77 °F), 45 days, 1 M KCl)

9.3 Process

9.3.1 Process temperature

0 to 140 °C (32 to 280 °F)

9.3.2 Process pressure

0 to 6 bar (0 to 87 psi)

9.3.3 Minimum conductivity

50 µS/cm

9.3.4 pH range

-2 to 14 pH

9.4 Mechanical construction

9.4.1 Weight

600 g (1.3 lbs)

9.4.2 Material

Sensor body:	Glass-lined steel, chemically resistant and shock resistant
Adapter and terminal head:	Stainless steel 1.4404 (AISI 316 L), PVDF, PTFE
Electrolyte vessel:	Stainless steel 1.4301 (AISI 304)
Process connections:	Stainless steel 1.4404 (AISI 316 L)

9.4.3 Process connections

M20

Pg 13.5

3/4"

1"

Nozzle DN25

Nozzle DN30

Varivent DN50/40

Sanitary fitting DN50

Sanitary fitting DN25

Tri-Clamp DN50

9.4.4 Temperature sensor

NTC 30K Ω

9.4.5 Reference system

Ag/AgCl with 3 M KCl and inhibitor (1 ml/l colloidal silicic acid)

Index

A

Approvals 6

C

Calibration 18
Changing the electrolyte 19
Cleaning 21–22
Commissioning 4, 14
Connection
 Electrolyte monitor 13
 Sensor 12

D

Description of the sensor 7
Designated use 4
Dimensions 9
Disinfecting the electrolyte system 14
Disinfection 14
Disposal 25

E

Electrical connection 12
Electrolyte monitor
 Connection 13
Environment
 Ambient temperature 26
 Storage temperature 26

F

Filling the electrolyte vessel 16

I

Icons 5
Identification
 Approvals 6
 Nameplate 6
Input
 Measured variables 26
 Measuring range 26
Installation 4, 7
 Dimensions 9
 Electrolyte monitor 11
 Electrolyte vessel 10
 Orientation 8
 Process 10

M

Maintenance 19
Material 27
Measured variables 26
Measuring range 26
Mechanical construction
 Material 27
 Process connections 27
 Reference system 27
 Temperature sensor 27
 Weight 27
Minimum conductivity 26

N

Nameplate 6

O

Operation 4
Operational safety 5

P

Process conditions
 Minimum conductivity 26
 pH range 26
 Process pressure 26
 Process temperature 26
Process connections 27

R

Reference system 27
Regeneration 15

S

Safety
 Commissioning 4
 Designated use 4
 Icons 5
 Installation 4
 Operation 4
 Operational safety 5
Sensor
 Calibration 18
 Cleaning 21–22
 Connection 12
 Disinfecting the electrolyte system 14

Filling the electrolyte vessel 16
Regeneration 15
Sterilization 21–22
Spare parts 25
Sterilization 21–22
Storage temperature 26

T

Technical data 26
Temperature sensor 27
Troubleshooting 25
Troubleshooting instructions 25
Types of calibration 18

U

Use 4

W

Weight 27
Wiring 12

Declaration of Hazardous Material and De-Contamination

RA No.

--	--	--	--	--	--	--	--

Please reference the Return Authorization Number (RA#), obtained from Endress+Hauser, on all paperwork and mark the RA# clearly on the outside of the box. If this procedure is not followed, it may result in the refusal of the package at our facility.

Because of legal regulations and for the safety of our employees and operating equipment, we need the "Declaration of Hazardous Material and De-Contamination", with your signature, before your order can be handled. Please make absolutely sure to attach it to the outside of the packaging.

Type of instrument / sensor _____ Serial number _____

☐ Used as SIL device in a Safety Instrumented System

Process data

Temperature _____ [°F] _____ [°C]
Conductivity _____ [µS/cm]

Pressure _____ [psi] _____ [Pa]
Viscosity _____ [cp] _____ [mm²/s]

Medium and warnings

								
	Medium /concentration	Identification CAS No.	flammable	toxic	corrosive	harmful/irritant	other *	harmless
Process medium								
Medium for process cleaning								
Returned part cleaned with								

* explosive; oxidising; dangerous for the environment; biological risk; radioactive

Please tick should one of the above be applicable, include safety data sheet and, if necessary, special handling instructions.

Description of failure

Company data

Company _____	Phone number of contact person _____
Address _____	Fax / E-Mail _____
_____	Your order No. _____

"We hereby certify that this declaration is filled out truthfully and completely to the best of our knowledge. We further certify that the returned parts have been carefully cleaned. To the best of our knowledge they are free of any residues in dangerous quantities."

(place, date)

Name, dept. (please print)

Signature

For more Endress+Hauser product please visit: www.ainstru.com

Mail: Sales@ainstru.com

www.endress.com/worldwide

Endress+Hauser 
People for Process Automation

BA468C/07/EN/06.10
FM9

