

Technical Information

Proservo NMS5

Intelligent Tank Gauge with High Accuracy
Performance Liquid Level, I/F, Density & Density
Profile Application



Application

Proservo NMS5 of intelligent tank gauges is designed for high accuracy liquid level measurement in storage and process applications.

It fulfills the exact demands of tank inventory management, loss control, total cost saving and safe operation.

Typical areas of application include:

- Oil (fuels), LPG/LNG, Chemicals, Water / chemical interface measurement Alcohols
- Tank mounted intelligence makes the NMS5 ideal for single or multi-task installation, converting a wide range of measurement functions including:
- Liquid level, Interface level, Spot density, Density profile, Tank bottom, Water Drop

Features and Benefits

- SIL2 Certified
- Measures liquid to an accuracy of ± 0.7 mm
- Measures two clear interface levels and specific gravity of up to three liquid phases
- Profiling of liquid density throughout the tank (Tank profile) and upper layer (I/F profile)
- Latest microtechnology keeps the design simple, lightweight and compact
- Wetted parts are completely separated from the electronic circuit
- Tank top mounting with 3" flange weighing only 12kg (aluminum version)
- Wide range of output signals including V1, RS 485, WM550, M/S, Enraf BPM and HART protocol
- Material and pressure rating of the wetted parts can be selected according to the application.
- Suitable for atmospheric and high pressure applications up to 2.45MPa/24.5bar
- Maintenance prediction of the instrument
- Direct connection of spot or average temperature probes
- Easy to program using the E+H matrix system
- Robust IP67/NEMA 4X housing
- Selectable English, Japanese or Chinese display
- Proactive safety diagnostics output to display and System Operators (patent pending)

Table of Contents

Important Document Information	3	Operating Conditions: Environment	23
Notes on Safety Conventions and Symbols	3	Ambient Temperature	23
Function and System Design	4	Storage Temperature	23
System Design	4	Liquid Temperature	23
System Configuration	5	Degree of Protection	23
Major Application	5	Electromagnetic Compatibility (EMC)	23
Operating Principle	6	Operating Condition: Process	24
Typical Tank Installation	7	Process Pressure	24
Measurement Terminology	8	Measuring Range	24
Application Selection	9	Mechanical Construction	25
Displacer Selection Guide	9	Design and Dimensions	25
Displacer Types	9	Housing Materials of Construction	26
Recommended Displacer by Application	9	Weight	26
Point to Confirm	10	Flange Type	26
Custody Transfer	10	Measuring Wire	26
Material Compatibility	10	Displacer	26
Process Connection Size	10	Cable Entry	26
Input and Output	11	Human Interface	27
Input for Local Devices	11	Operating Concept	27
Output Parameters based on Communication Protocol	11	Display (LCD)	27
RS485 Modbus	12	Programming	27
Bidirectional Serial Pulse (V1 Protocol)	12	Memo Function	27
HART Protocol	12	Advanced Maintenance	28
Whessoematic 550	13	Maintenance Prediction	28
Mark/Space	13	Maintenance	28
Enraf Bi Phase Mark (BPM)	13	Proactive Safety	28
Analogue Output	14	Certificates and Approval	29
Relay	14	CE Mark	29
Auxiliary Energy (Wiring for Primary Output)	16	Ex Approvals	29
V1 Serial Pulse Modbus RS 485HART Enraf BPM	16	Custody Transfer Approvals	29
Whessoematic 550	17	Overspill Prevention	29
Mark/Space	18	SIL2	29
Cable Entry	19	External Standards and Guidelines	29
Overvoltage Protection	19	Order Information	30
Supply Voltage	19	NMS5	30
Power Consumption	19	Accessories	33
Safe Electrical Isolation	19	Calibration Chamber	33
Performance Characteristics	20	Power + Control Switch	35
Maximum Measured Error	20	Ball Valve	36
Compensation	20	Reducing Flange	38
Operating Conditions: Communications	21	Supplementary Documentation	39
Modbus (RS485 Output)	21	Technical Information	39
Sakura V1 Serial Pulse Output	21	Operating Manual	39
Enraf Bi Phase Mark Output	21	Compact Instructions	39
HART Output	22	Safety Instructions	39
Whessoematic 550 (WM 550) Output	22	Functional Safety Manual	39
Varec Mark Space(M/S) Output	22	Appendix	40
		Stainless Steel Conversion Table	40

Important Document Information

Notes on Safety Conventions and Symbols

Symbols for Safety Conventions

Symbol	Meaning
 DANGER A0011189-EN	DANGER! This symbol alerts you to a dangerous situation. Failure to avoid this situation will result in serious or fatal injury.
 WARNING A0011190-EN	WARNING! This symbol alerts you to a dangerous situation. Failure to avoid this situation can result in serious or fatal injury.
 CAUTION A0011191-EN	CAUTION! This symbol alerts you to a dangerous situation. Failure to avoid this situation can result in minor or medium injury.
 NOTICE A0011192-EN	NOTICE! This symbol contains information on procedures and other facts which do not result in personal injury.

Symbols for Certain Types of Information

Symbol	Meaning
 A0011182	Allowed Indicates procedures, processes or actions that are allowed.
 A0011183	Recommendation Indicates procedures, processes or actions that are recommended.
 A0011184	Forbidden Indicates procedures, processes or actions that are forbidden.
 A0011193	Tip Indicates additional information.

Function and System Design

System Design

NMS5 is an intelligent tank gauge for measuring liquid levels with high precision, and employing the latest microprocessor technology. In addition to gauging level, NMS5 can measure the interfaces between up to three liquids, density, and tank bottom. To enable accurate volume calculation or simple indication, NMS5 will accept input from either an average temperature probe NMT 53x series (via twisted pair cables, HART protocol) or spot temperature element (via 3 wire Pt. 100 RTD signal). Once installed, all calibration and operating functions can be done via the user friendly Matrix program and touch sensitive keypad. Tank side monitoring and liquid measurement operation can be performed by the Promonitor NRF560.

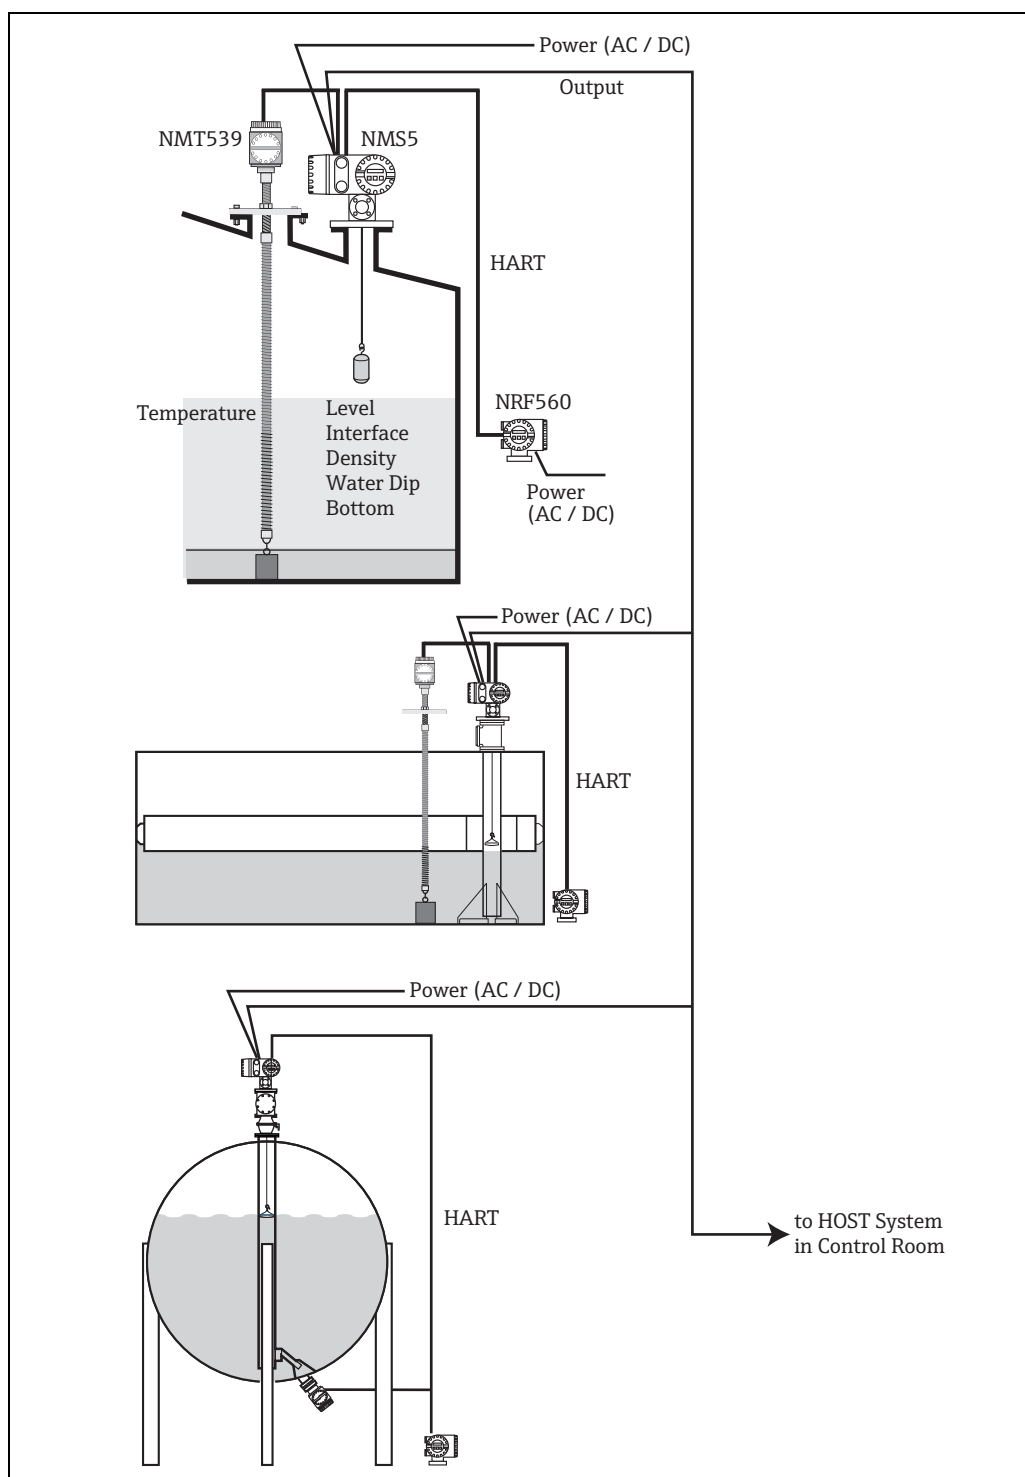


Figure 1: Measuring System

System Configuration

- From single tank level measurement to the largest oil refinery applications, NMS5 can be an integral part of tank farm management solutions. A wide variety of data output protocols are available for seamless integration into many commonly used systems.
- A primary example is Endress+Hauser's revolutionary Tankvision., A scalable concept, offering local tank management for up to 225 tanks via Modbus, V1 or Whessomatic 550 protocols. Accumulated data is available to DCS and other plant management systems via a Host Link.
- Output protocols
 - Modbus, RS485 or current loop
 - V1 serial pulse
 - Whessomatic 550
 - local HART
 - Mark/Space
 - Enraf BPM

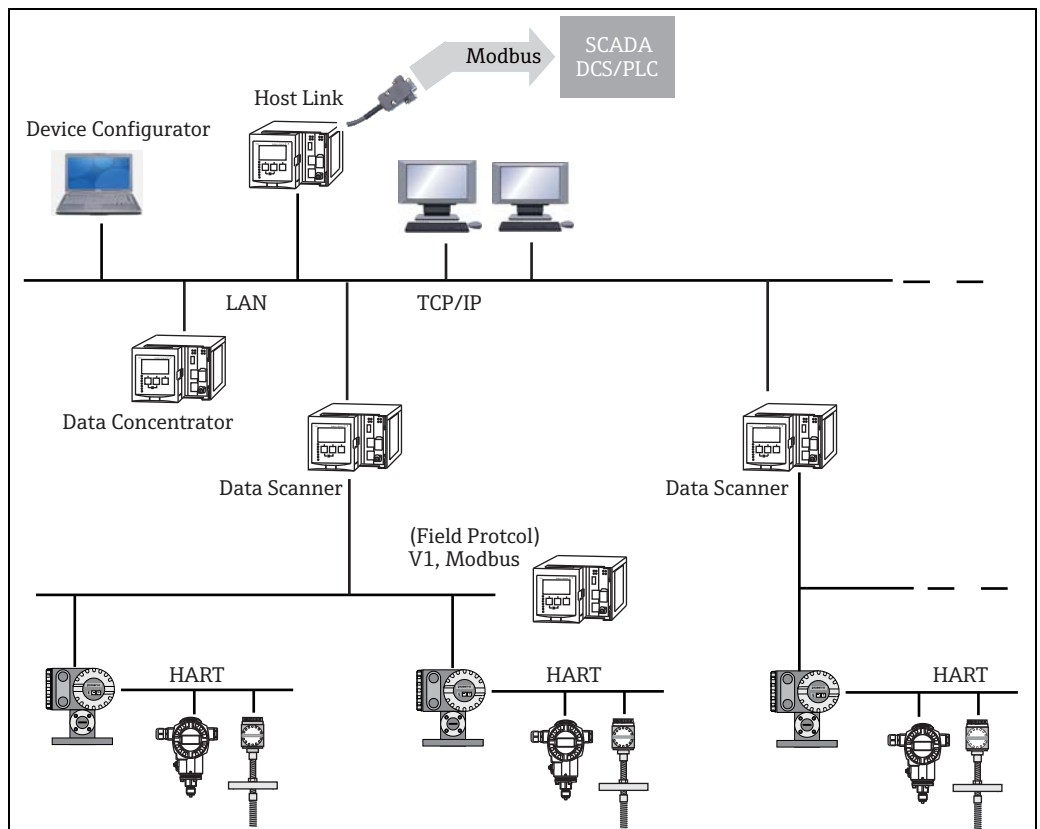


Figure 2: NMS5 system configuration Serial pulse output

Major Application

The number of measuring functions and output options as well as the lightweight compact design enables NMS5 to be installed in a wide range of applications at minimal cost.

Petroleum Industry

From oil production to storage at an oil depot, there exists an extensive need to measure and manage a wide variety of products. Remote tank gauging and an inventory management system combined into NMS5 and a receiving computer is an ideal way to measure and manage tank contents.

Chemical Industry

A wide choice of products are available in the wetted parts construction manufacturing industry, to ensure chemical compatibility and long life.

Power Plant

Oil levels are a major applications where precise measurement is required to ensure safe operation.

Operating Principle

A small displacer is accurately positioned in a liquid medium using a servo motor. The displacer is then suspended on a measuring wire which is wound onto a finely grooved drum housing. NMS5 counts the rotation of the wire drum and calculates the traveling distance of the wire and then obtain the liquid level change. The drum is driven via coupling magnets which are completely separated by the drum housing. Outer magnets are connected to the wire drum whilst inner magnets are connected to the drive motor. As the inner magnets turn, their magnetic attraction causes the outer magnets to turn, as well, causing the entire drum assembly to turn. The weight of the displacer on the wire creates torque on the outer magnets generating change of magnetic flux. These changes generated in the drum assembly are detected by a unique electromagnetic transducer on the inner magnets. The drive motor is actuated to balance the voltage generated by variations of magnetic flux to equal the reference voltage defined by operating commands. When the displacer is lowered and touches a liquid, the weight of the displacer is reduced by liquid buoyancy force. As a result, torque in the magnetic coupling changes, which is measured by 5 sets of Hall sensors, (patented) chips which are temperature compensated. A signal, indicating the position of the displacer, is sent to the motor control circuit. As the liquid levels rise and fall, the displacer position is adjusted by the drive motor. The rotation of the wire drum is precisely evaluated to determine level value.

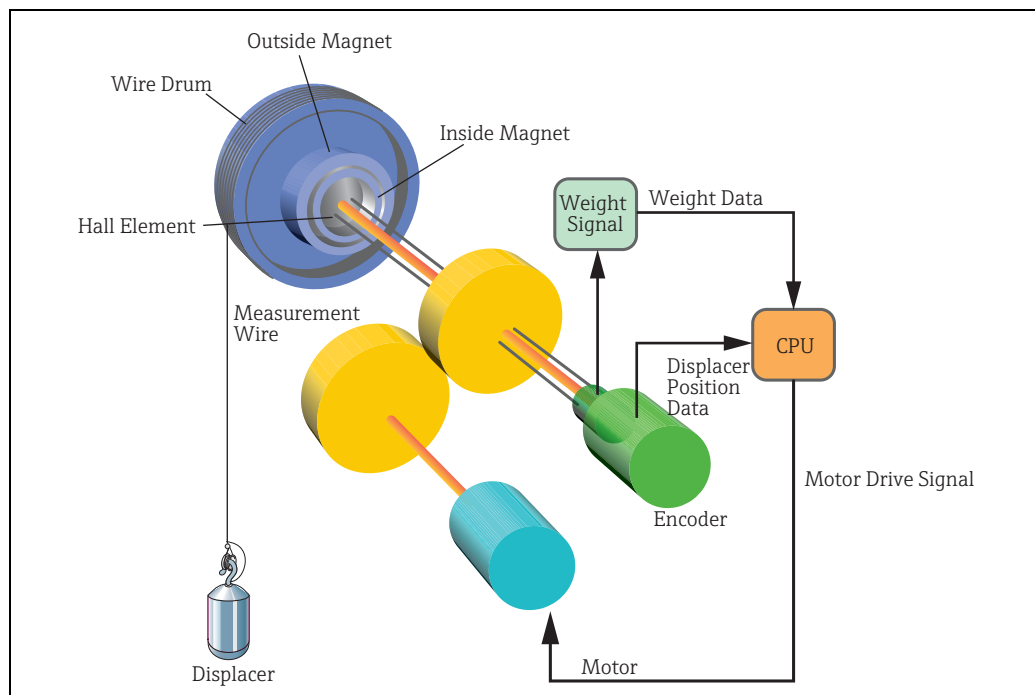


Figure 3: Direct Torque Detection

Typical Tank Installation

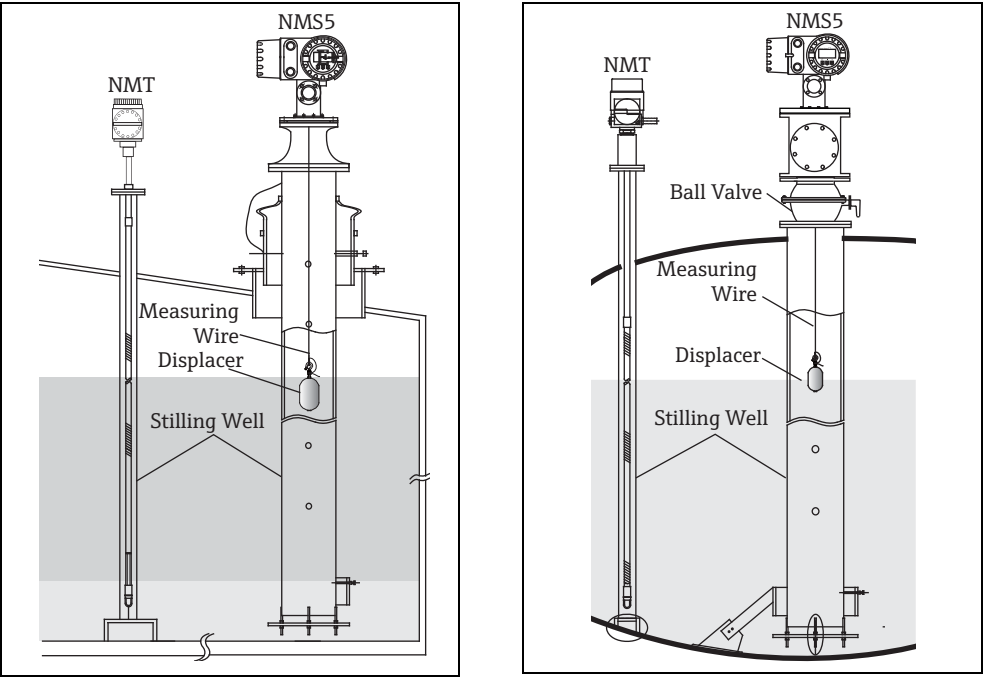


Figure 4: Fixed Roof Tank (Left) / High Pressure Tank (Right)

Floating Roof Tank/
Covered Floating Roof Tank

CAUTION
When installing NMS5 to floating roof tank,
make sure to use stilling well.

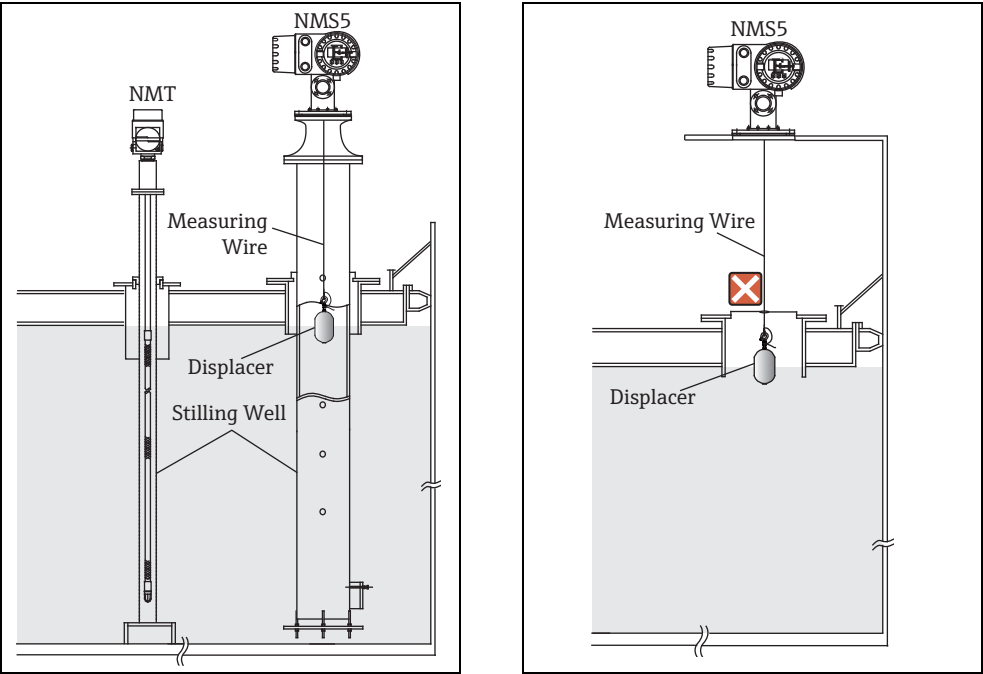


Figure 5: Floating Roof Tank

Measurement Terminology

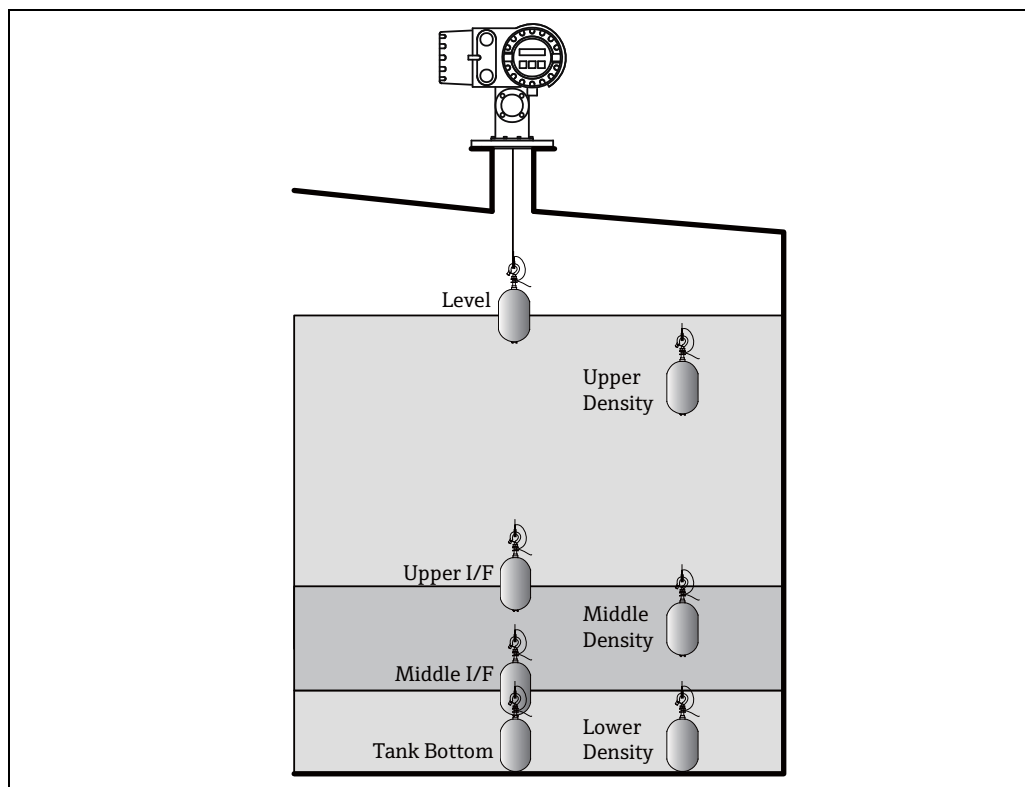


Figure 6: NMS5 with standard level, I/F x 2, Tank bottom and spot density x 3 measurement

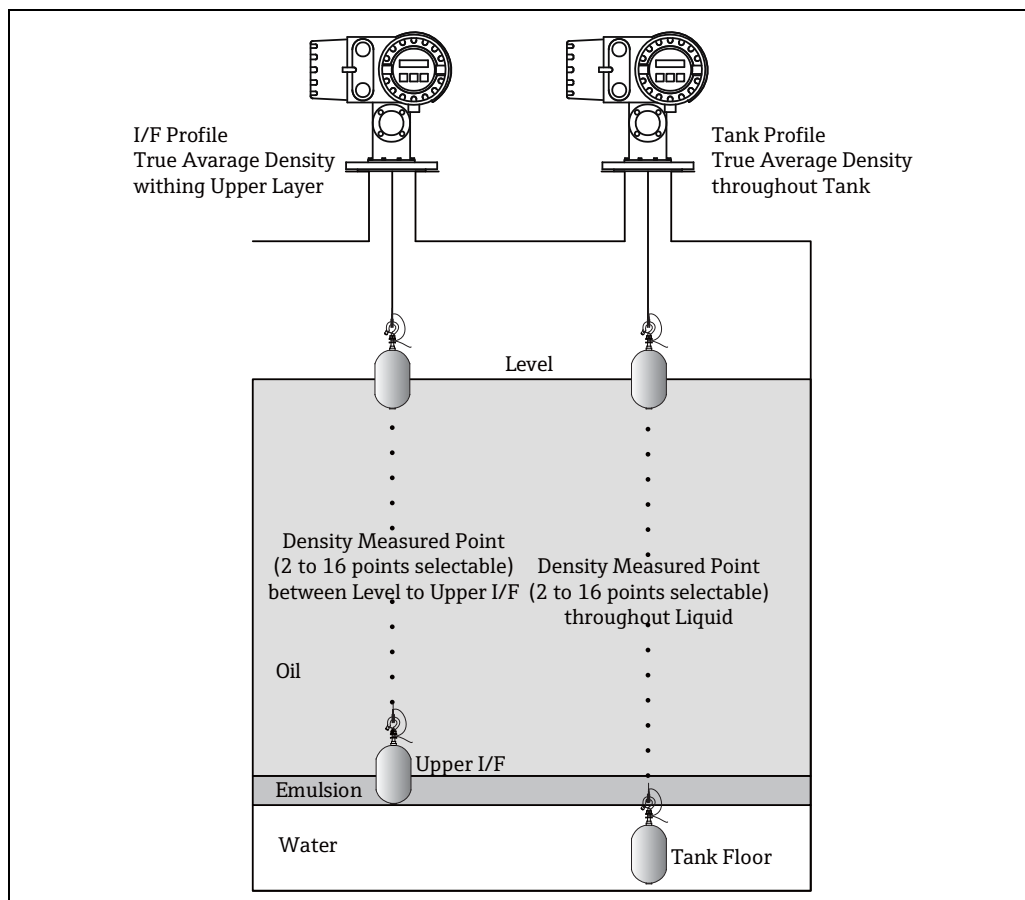

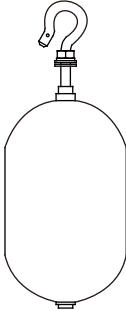



Figure 7: Density Profile measurement "I/F (Interface) Profile" (Left) "Tank Profile" Measurement Range (Right)

Application Selection

Displacer Selection Guide A wide variety of displacers are available to meet your applications. Proper displacer selection ensures optimal performance and longevity. The following guidelines will assist you in selecting the ideal displacer for your application.

Displacer Types

30mm	40mm	50mm	70mm	110mm
SUS316/PTFE	SUS316/PTFE	SUS316/PTFE Alloy C	SUS316	SUS316
				
(Standard materials available)				

Recommended Displacer by Application

Application	Surface	Interface	Density
Viscous	50mm PTFE	Not Recommended	Not Recommended
Crude	50mm 316 50mm PTFE	50mm 316 50mm PTFE	50mm 316 50mm PTFE
Black oil	50mm 316	50mm 316	50mm 316
White oil	50mm 316	50mm 316	50mm 316
Liquefied gases, LPG/LNG	70mm 316	70mm 316	50mm 316
Aggressive	50mm Alloy C 50mm PTFE	50mm Alloy C 50mm PTFE	50mm Alloy C 50mm PTFE
Custody Transfer	70mm 316 110mm 316	N/A	N/A

NOTICE
The above table is for 80A (3") mounting flange or larger.

Point to Confirm**Application:**

What will be the primary measurement function in your application? Most applications can be generalized into three classifications: level data, density data, or both. NMS5 is primarily a highly accurate level measurement gauging instrument, with the added ability to measure density. Level is derived by determining fluid surface level, interface level(s) between different liquids, as well as finding tank floor or datum plate. Density served from single-point (called “spot” measurements), as well as profile measurements of all liquid(s) in a tank.

Surface Level:

In general, larger diameter displacers have better accuracy under similar conditions.

Interface Level(s):

Cylindrical-shaped displacers, with rounded top and bottom, reduce resistance while moving through liquid(s). Thus, providing smoother movement and faster interface measurements, compared to flat-based displacers, particularly in density profile measurements that span the full tank height.

⚠ CAUTION

Note that in order for a displacer to travel down through liquid(s), displacer density (its weight divided by its volume) must be higher than liquid(s) density.

Tank-bottom/Datum Plate Level:

(same as for Interface Levels)

Density:

Since the density is the calculated result of two of more measurements, a displacer with higher volume will usually yield the most accurate density measurement. In most cases we recommend our 50mm diameter displacer for density measurement.

Level and Density:

When an application calls for equal importance placed on measuring both level and density, the 50mm diameter, cylindrical displacer will give the best all-around performance.

Custody Transfer

What is the requirement for Custody Transfer approval?

- The 70mm, conical, 316 displacer is the choice for requirements per NMI
- The 110mm, conical 316 displacer is the choice for requirements per PTB

Material Compatibility

What are the liquid(s) characteristics of your application? Displacers are available in three different standard materials. Material compatibility should be confirmed to ensure safe operation and optimal NMS5 performance.

316:

Stainless steel is a highly versatile industrial material and provides good compatibility with a wide range of chemicals, including most white and black oils.

Alloy C:

This high-performance material is harder than 316, and provides excellent resistance to many of harshest corrosive chemical applications.

PTFE:

One of the most well-known and versatile polymer materials, this high-performance material has one of the lowest friction coefficients. It provides excellent performance in viscous/sticky liquids, and also has excellent chemical resistance to a wide range of corrosives

Process Connection Size

The process connection defines the tank process entry, and may affect displacer size. The standard NMS5 process connections start at 3”/DN80 and fit most tank gauging applications. Accordingly, most applications can be covered with one of the 50mm or 70mm displacer options. Smaller diameter displacers are available when the process connection is smaller.

⚠ CAUTION

Note that, when the 110mm diameter custody transfer approval (PTB) displacer is selected, a separate calibration and maintenance chamber is recommended between the NMS5 and tank process connection.

Input and Output

Input for Local Devices

Signal	Multi drop local HART protocol max. 4 devices
Power supply	DC 24V
Additional units	NMT 53x average temperature sensor NRF 560 field data processor Other - compatible HART devices Spot temperature Pt 100 Ohm ISO standard three wire connection

Output Parameters based on Communication Protocol

	V1(new)	V1 (old)	MODBUS	HART	WM550	ENRAF	M/S
Level	Yes	Yes	Yes	Yes	Yes	Yes	Yes
Temperature (Product)	Yes	Yes	Yes	Yes	Yes	Yes	Yes
Vapor Temperature	Yes	-	Yes	Yes	Yes	-	-
Upper I/F (Water Level) *1	Yes	-	Yes	Yes	Yes	Yes	-
Middle I/F	Yes	-	Yes	Yes	-	-	-
Upper Density *2	Yes	-	Yes	Yes	Yes	-	-
Middle Density*3	Yes	-	Yes	Yes		-	-
Lower Density*4	Yes	-	Yes	Yes		-	-
Average Density *5	Yes	-	Yes	-	Yes	-	-
1-16 points Individual Density *6	Yes	-	Yes	-	-	-	-
Multi-Element Temperature	Yes	-	Yes	Yes	Yes	--	-
HART device input (Device 1)	Yes	-	Yes	Yes	Yes	-	-
HART device input (Device 2)	Yes	-	Yes	Yes	Yes	-	-
Alarm data	Yes	Yes	Yes	Yes	Yes	Yes	-
Protocol Documentation	-	-	KA0002N	-	KA001N	-	-

CAUTION

- *1. Upper I/F output value can be either selected from the Proservo's own displacer measurement or Water Bottom measured value via the Prothermo NMT 539.
- *2. A single point density measurement within the upper layer liquid in the tank. The measurement position is configured to 150mm below the liquid surface at default.
- *3. A single point density measurement within the middle layer liquid in the tank. The measurement position is configured to 150mm below the upper interface level at default.
- *4. A single point density measurement within the lower layer liquid in the tank. The measurement position is configured to 150mm below the middle interface at default.
- *5. The value of this "Average Density" is based on the calculation after performing the Density Profile operation at NMS5.
- *6. All of the selected number of density measured value from 1 to 16 points can be transmitted.

RS485 Modbus

Module name	Commdule RS 485 communication module (until 2008), COM - 5 (from 2009)
No. of unit	Maximum 10 instruments per loop
Baud rate	600/1,200/ 2,400/ 4,800/ 9,600/ 19,200 bit/s, selectable
Parity	Odd, Even, None, selectable
Cable	Two wire twisted cable with screening (DGND is connected to the ground cable)
Topology	Serial bus, electrically isolated, tree structure
Transmission distance	Maximum 1,200 m including limbs or branches (negligible with branches under 3 m)
Instrument address	Accessed via touch control
Isolation	Bus inputs are electrically isolated from the other electronics

Bidirectional Serial Pulse (V1 Protocol)

Module name	COM - 1
No. of units	Maximum 10 instruments per loop
Baud rate	3,300 BPS
Cable	Two wire (twisted pair) unscreened cable
Topology	Serial bus, tree structure
Transmission distance	Maximum 6,000 m
Instrument address	Accessed via touch control
Isolation	Serial communication circuit isolated from other circuits

HART Protocol

Module name	Commdule HART (from 2009), COM - 6 (from 2009)
No. of units	Maximum 15 instruments per loop
Baud rate	1,200 BPS
Cable	Two wire, twisted pair screened cable Minimum core ϕ 0.15 (24AWG)
Transmission distance	Maximum 1,200 m
Instrument address	Accessed via touch control or HART master device
Isolation	Bus input are electrically isolated from the other electronics

Whessoematic 550

Module name	WM550 communication module
No. of units	15 instruments per loop (connected to RTU)
Baud rate	1,200 / 2,400 bit/s
Cable	Two wire, twisted cable with screening
Topology	20 mA current loop
Transmission distance	Depending on specifications (ask your E+H engineer)
Instrument address	Setting by DIP switches on communication board
Isolation	Current loop circuit isolated from other circuits

Mark/Space

Module name	Mark/Space communication module
No. of units	Depending on specification (ask to your E+H engineer)
Baud rate	1,200 / 2,400 / 4,800 / 9,600 / 19,200 bit/s
Cable	Four wire
Topology	Serial bus, tree structure
Transmission distance	Depending on specifications (ask your E+H engineer)
Instrument address	Setting by DIP switches on communication board
Isolation	Serial pulse isolated from other circuits

Enraf Bi Phase Mark (BPM)

Module name	COM - 3
No. of units	Maximum 10 instruments per loop
Baud rate	1,200, 2,400 bit/s, selectable
Cable	Two wire, twisted cable with screening
Topology	Serial bus, electrically isolated, tree structure
Transmission distance	Maximum 10 km
Instrument address	Accessed via touch control
Isolation	Serial communication circuit isolated from other circuits

Analogue Output

Module name	I/O - 5
Output	4 to 20 mA, active
On alarm	Switchable Max. 22mA, Min. 2mA or hold last measured value
Electrical isolation	Analogue output isolated from other circuits
Maximum load	500 ohm
Conversion Accuracy	+/-0.3%

Relay

Module name	I/O - 3		
Alarm output, Standard (Order Code position 050= 1,2,3 or 5)	4 relays with potential-free change-over contacts, freely assignable to measured value		
Hysteresis, Alarm output	Switch points and switching hysteresis freely adjustable, residual current fail-safe mode: minimum or maximum, selectable		
Operation output logic		Relay Condition	
	Initial Configuration (Normal Status)	Open	Closed
	On alarm	Closed	Open
	On device error	Closed	Open
	On abnormal power supply (5% lower than, higher than specified power supply)	Custody Transfer Closed	Custody Transfer Open
	Power outage	Hold last condition	
Switching capacity, Alarm output	</		

Alarm output, Overspill prevention (Order Code position 050=4)	2 relays with potential- free changeover contacts, assignable to Level	
Hysteresis, Alarm output	Switch points and switching hysteresis freely adjustable, residual current fail-safe mode: minimum or maximum, selectable	
Operation output logic		Relay Condition
	Initial Configuration (Normal Status)	Closed
	On alarm	Open
	On device error	Open
	On abnormal power supply (5% lower than, higher than specified power supply)	Open
	Power outage	Open
Switching capacity	▪ Umax. 200VDC/200VppAC ▪ Imax. 0.5AC, DC or peak AC ▪ Pmax. 15W	


NOTICE

When selecting Output2: "4: 2 x relay SPST, TUV with overspill prevention" at order code 50, relay type is specified as only Normal Closed.

Operation Input	2 photocouplers, for external input from controller (tumbler switch, DCS, etc.)		
Operation output logic	Gauge Status	CTR1	CTR2
	Level	0 (OFF)	0 (OFF)
	UP	1 (ON)	0 (OFF)
	STOP	0 (OFF)	1 (ON)
	Interface Level	1 (ON)	1 (ON)
Input voltage	15VDC, active circuit (supplied by NMS5)		
Input current	Approximately 5mA		

Auxiliary Energy (Wiring for Primary Output)

V1 Serial Pulse, Modbus RS
485, HART Enraf BPM

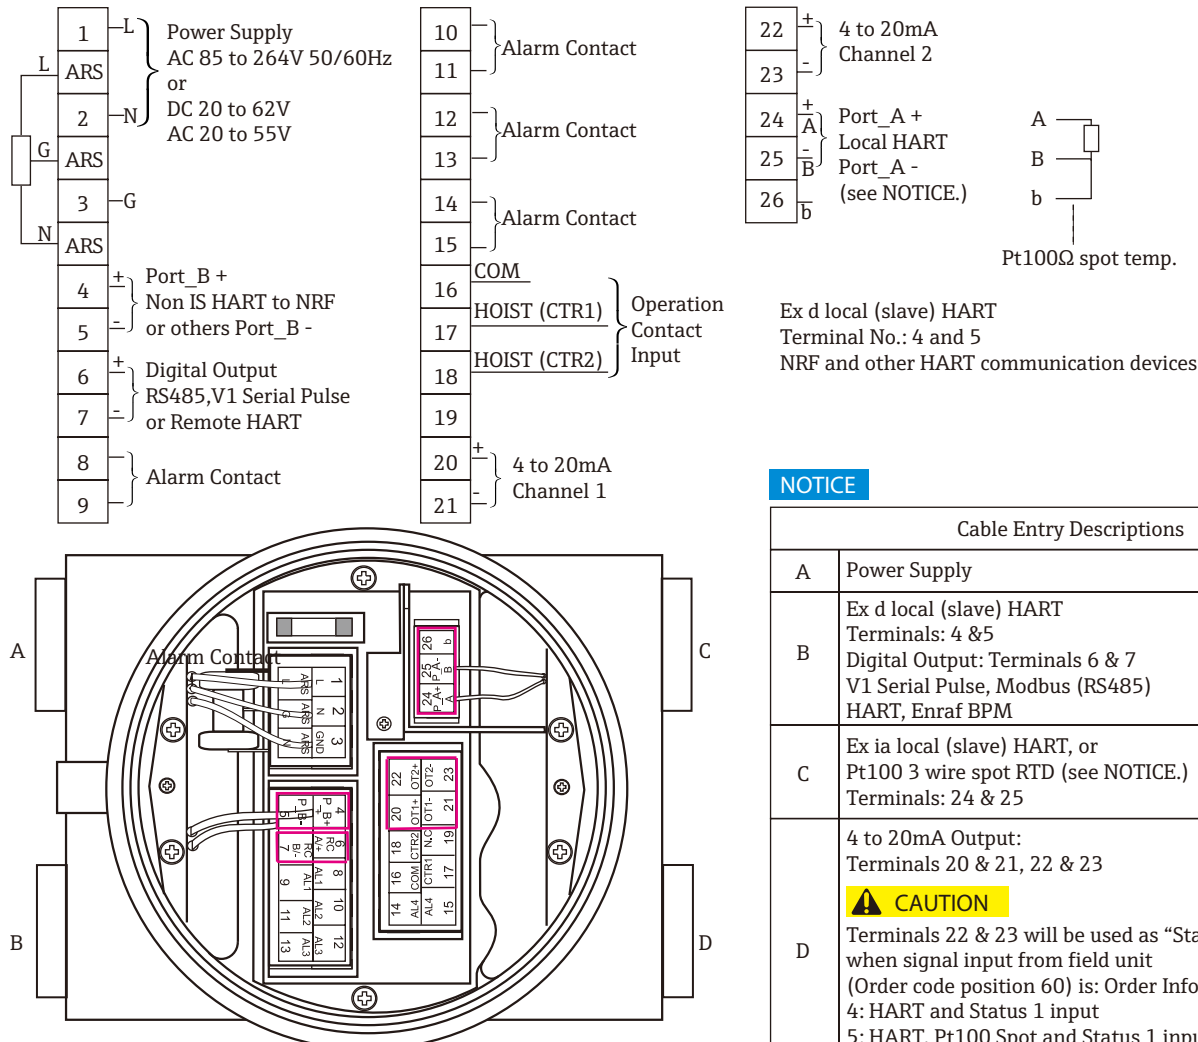

NOTICE

Cable Entry Descriptions	
A	Power Supply
B	Ex d local (slave) HART Terminals: 4 & 5 Digital Output: Terminals 6 & 7 V1 Serial Pulse, Modbus (RS485) HART, Enraf BPM
C	Ex ia local (slave) HART, or Pt100 3 wire spot RTD (see NOTICE.) Terminals: 24 & 25
D	4 to 20mA Output: Terminals 20 & 21, 22 & 23 CAUTION Terminals 22 & 23 will be used as "Status 1 Input" when signal input from field unit (Order code position 60) is: Order Information: 060 4: HART and Status 1 input 5: HART, Pt100 Spot and Status 1 input 6: HART, Pt100 Spot temp., Operation contact, and Status 1 input

NOTICE

- Terminal connection for Whessoe Matic 550 (WM550) and Mark Space, refer to the next few pages.
- Terminals 4 & 5 and 24 & 25 for HART devices are inter - connected on Explosion proof (Ex d) certified version.
- Terminals 24 & 25 (and 24, 25 & 26 for spot temp.) will be intrinsically safe (i.s.) device connection only when intrinsically safe certified version is selected.

Figure 8: Wiring Sample 1

Whessoematic 550


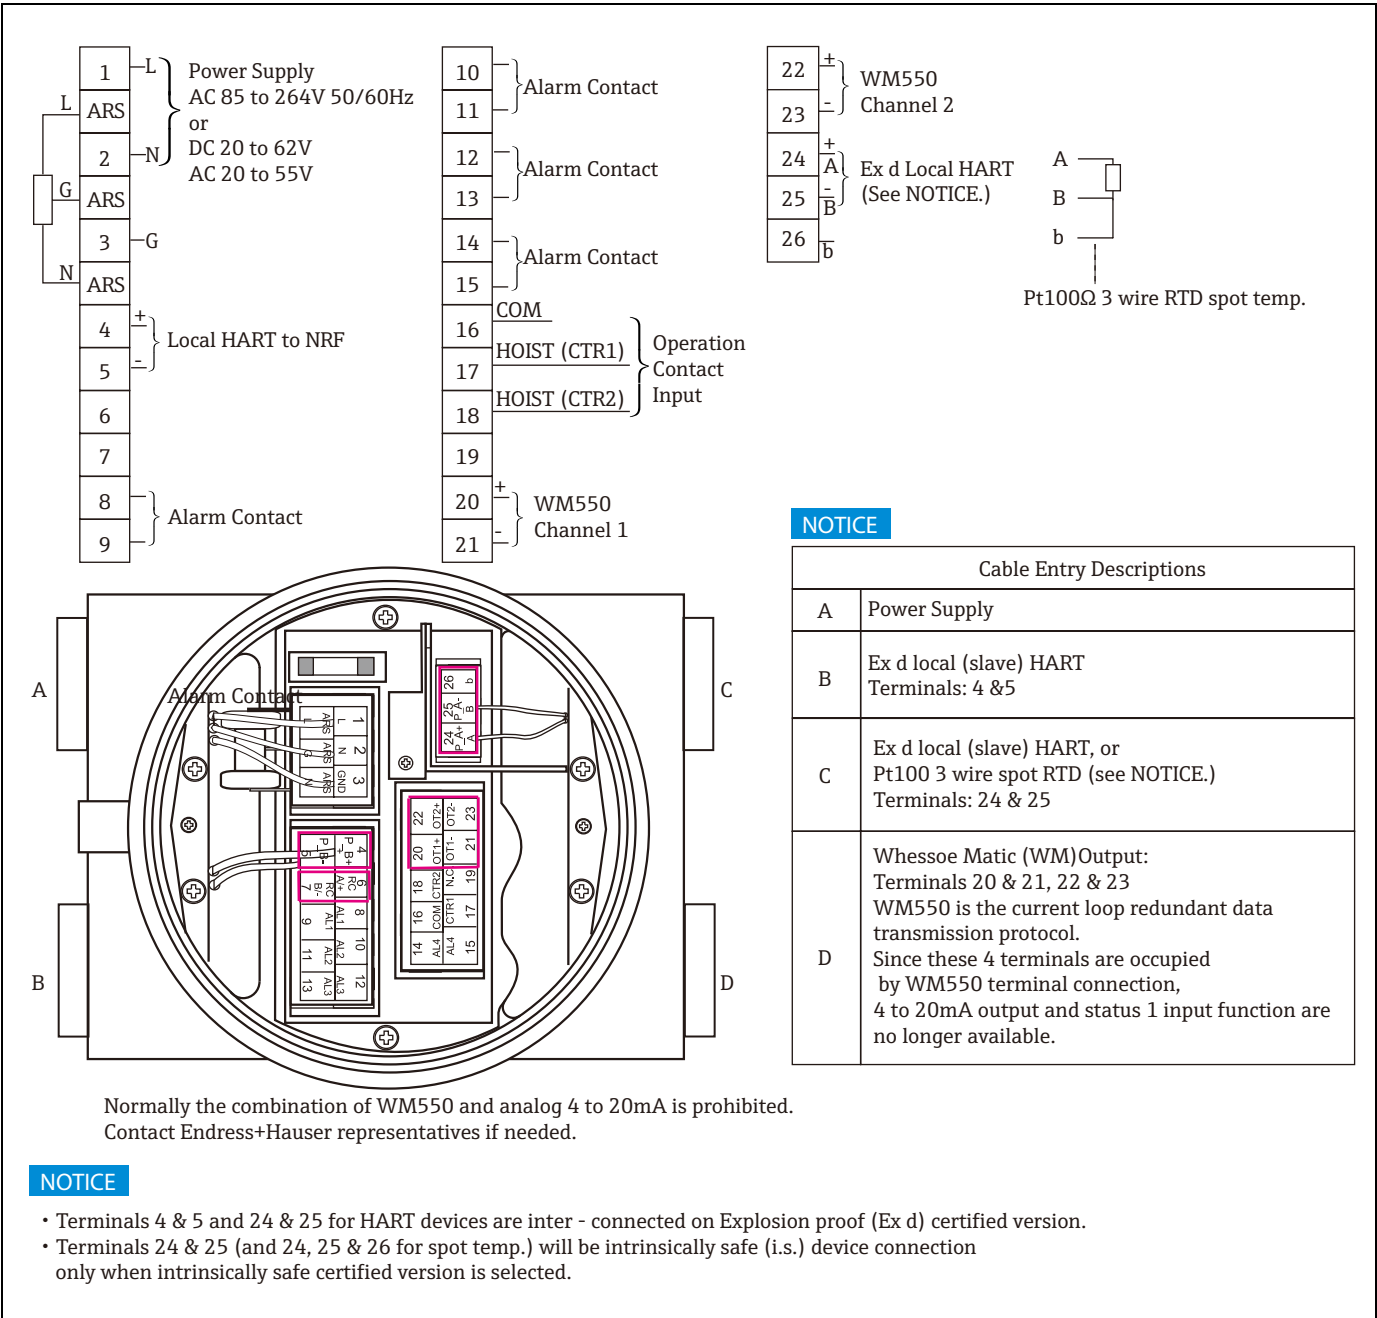


Figure 9: Wiring Sample 2

Mark/Space

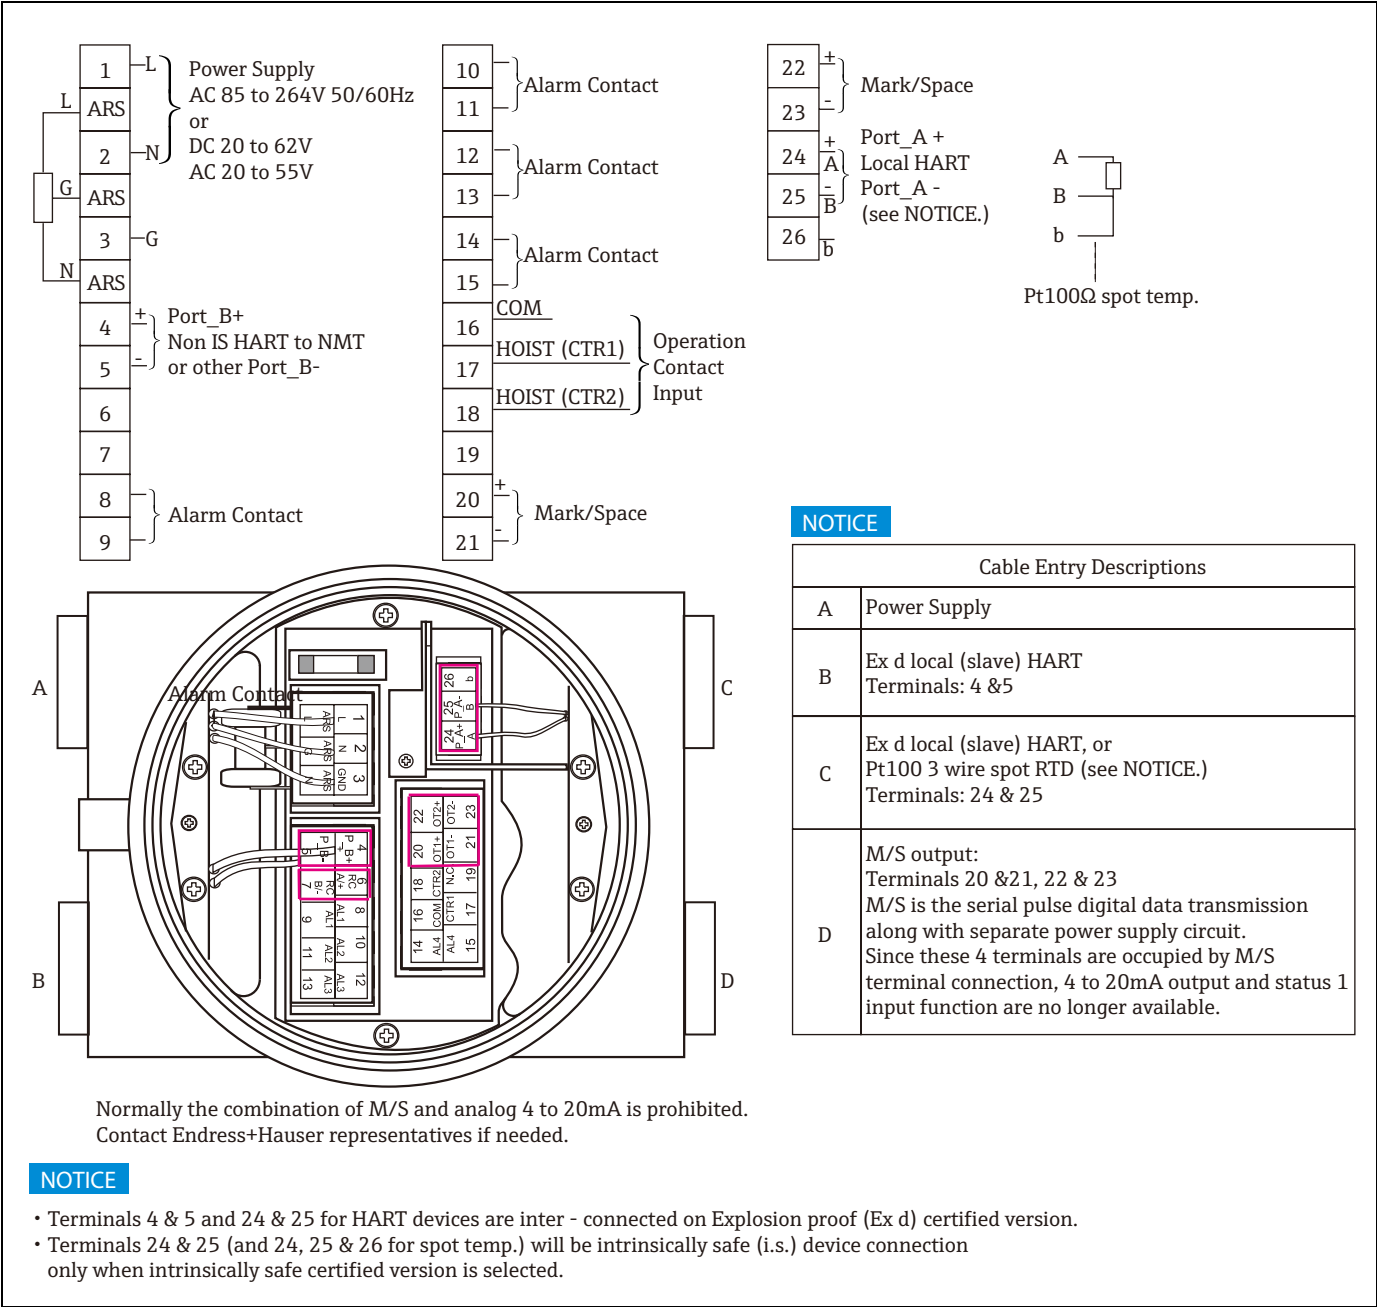

A

B

C

D

Alarm Contact

1

2

3

4

5

6

7

8

9

10

11

12

13

14

15

16

17

18

19

20

21

22

23

24

25

26

27

28

29

30

31

32

33

34

35

36

37

38

39

40

41

42

43

44

45

46

47

48

49

50

51

52

53

54

55

56

57

58

59

60

61

62

63

64

65

66

67

68

69

70

71

72

73

74

75

76

77

78

79

80

81

82

83

84

85

86

87

88

89

90

91

92

93

94

95

96

97

98

99

100

101

102

103

104

105

106

107

108

109

110

111

112

113

114

115

116

117

118

119

120

121

122

123

124

125

126

127

128

129

130

131

132

133

134

135

136

137

138

139

140

141

142

143

144

145

146

147

148

149

150

151

152

153

154

155

156

157

158

159

160

161

162

163

164

165

166

167

168

169

170

171

172

173

174

175

176

177

178

179

180

181

182

183

184

185

186

187

188

189

190

191

192

193

194

195

196

197

198

199

200

201

202

203

204

205

206

207

208

209

210

211

212

213

214

215

216

217

218

219

220

221

222

223

224

225

226

227

228

229

230

231

232

233

234

235

236

237

238

239

240

241

242

243

244

245

246

247

248

249

250

251

252

253

254

255

256

257

258

259

260

261

262

263

264

265

266

267

268

269

270

271

272

273

274

275

276

277

278

279

280

281

282

283

284

285

286

287

288

289

290

291

292

293

294

295

296

297

298

299

300

301

302

303

304

305

306

307

308

309

310

311

312

313

314

315

316

317

318

319

320

321

322

323

324

325

326

327

328

329

330

331

332

333

334

335

336

337

338

339

340

341

342

343

344

345

346

347

348

349

350

351

352

353

354

355

356

357

358

359

360

361

362

363

364

365

366

367

368

369

370

371

372

373

374

375

376

377

378

379

380

381

382

383

384

385

386

387

388

389

390

391

392

393

394

395

396

397

398

399

400

401

402

403

404

405

406

407

408

409

410

411

412

413

414

415

416

417

418

419

420

421

422

423

424

425

426

427

428

429

430

431

432

433

434

435

436

437

438

439

440

441

442

443

444

445

446

447

448

449

450

451

452

453

454

455

456

457

458

459

460

461

462

463

464

465

466

467

468

469

470

471

472

473

474

475

476

477

478

479

480

481

482

483

484

485

486

487

488

489

490

491

492

493

494

495

496

497

498

499

500

501

502

503

504

505

506

507

508

509

510

511

512

513

514

515

516

517

518

519

520

521

522

523

524

525

526

527

528

529

530

531

532

533

534

535

536

537

538

539

540

541

542

543

544

545

546

547

548

549

550

551

552

553

554

555

556

557

558

559

560

561

562

563

564

565

566

567

568

569

570

571

572

573

574

575

576

577

578

579

580

581

582

583

584

585

586

587

588

589

590

591

592

593

594

595

596

597

598

599

600

601

602

603

604

605

606

607

608

609

610

611

612

613

614

615

616

617

618

619

620

621

622

623

624

625

626

627

628

629

630

631

632

633

634

635

636

637

638

639

640

641

642

643

644

645

646

647

648

649

650

651

652

653

654

655

656

657

658

659

660

661

662

663

664

665

666

667

668

669

670

671

672

673

674

675

676

677

678

679

680

681

682

683

684

685

686

687

688

689

690

691

692

693

694

695

696

697

698

699

700

701

702

703

704

705

706

707

708

709

710

711

712

713

714

715

716

717

718

719

720

721

722

723

724

725

726

727

728

729

730

731

732

733

734

735

736

737

738

739

740

741

742

743

744

745

746

747

748

749

750

751

752

753

754

755

756

757

758

759

760

761

762

763

764

765

766

767

768

769

770

771

772

773

774

775

776

777

778

779

780

781

782

783

784

785

786

787

788

789

790

791

792

793

794

795

796

797

798

799

800

801

802

803

804

805

806

807

808

809

810

811

812

813

814

815

816

817

818

819

820

821

822

823

824

825

826

827

828

829

830

831

832

833

834

835

836

837

838

839

840

841

842

843

844

845

846

847

848

849

850

851

852

853

854

855

856

857

858

859

860

861

862

863

864

865

866

867

868

869

870

871

872

873

874

875

876

877

878

879

880

881

882

883

884

885

886

887

888

889

890

891

892

893

894

895

896

897

898

899

900

901

902

903

904

905

906

907

908

909

910

911

912

913

914

915

916

917

918

919

920

921

922

923

924

925

926

927

928

929

930

931

932

933

934

935

936

937

938

939

940

941

942

943

944

945

946

947

948

949

950

951

952

953

954

955

956

957

958

959

960

961

962

963

964

965

966

967

968

969

970

971

972

973

974

975

976

977

978

979

980

981

982

983

984

985

986

987

988

989

990

991

992

993

994

995

996

997

998

999

1000

Normally the combination of M/S and analog 4 to 20mA is prohibited.

Contact Endress+Hauser representatives if needed.

NOTICE

• Terminals 4 & 5 and 24 & 25 for HART devices are inter - connected on Explosion proof (Ex d) certified version.

• Terminals 24 & 25 (and 24, 25 & 26 for spot temp.) will be intrinsically safe (i.s.) device connection only when intrinsically safe certified version is selected.

Figure 10: Wiring Sample 3

Cable Entry	Thread: G1/2, 3/4 NPT1/2,3/4 M20, 25 *TIIS: G only, CSA: NPT only
Overvoltage Protection	NMS5 has internal surge arrester which complies with EN/IEC 61000-4-5 (Line to Line 1.0kV, Line to ground 2.0kV) Connect the metallic housing of the NMS5 to the tank wall or screen directly with an electrically conductive lead to ensure reliable potential matching.
Supply Voltage	High voltage type: 85 to 264 VAC, 50/60 Hz Low voltage type: 20 to 62 VDC / 20 to 55 VAC 50/60Hz  WARNING Allowable voltage supply is specifically stated depending on each Ex approval. Refer to the designated certification
Power Consumption	Maximum 50 VA, 50W
Safe Electrical Isolation	Between power supply and signal output, CPU, RS 485, relay and other electronics

Performance Characteristics

Maximum Measured Error

Level	$\pm 0.7\text{mm}$ ($\pm 0.027\text{ inch}$)* ¹
Interface	$\pm 2.7\text{ mm}$ ($\pm 0.106\text{ inch}$)* ²
Density	$\pm 0.005\text{ g/cm}^3$ (g/ml)* ³
Sensitivity	$\pm 0.1\text{ mm}$ ($\pm 0.004\text{ inch}$)

*¹ : Under reference conditions

*² : Difference of product densities 100kg/m^3 (g/ml) (6.25 lb/ft^3)

*³ : (optional) when calibrated and equipped for density measurement

Compensation

Displacer

Automatic compensation of displacer weight

Tank Wall

Compensation of depression and distortion

Operating Conditions: Communications

Modbus (RS485 Output)

Modbus is connected to Tankvision or other Modbus (RS485) receiver.

Termination Resistors

The terminal voltage for the device located at the furthest position from the receiver needs to be set with an NM5 that is connected on same line. The setting can be made using the mechanical dip switch on the communication board.

Bus Address

Each device has an individual bus address and can be set via touch control.

Bus Cabling

The bus cabling is galvanically isolated from the device or interface adapter. Standard communication cable (CPEV or KEPV) can be used for the data transmission.

Bus Topology

When planning a system, attention should be paid to possible segmentation of the bus according to individual plant sections. Suitable topologies are:

- Tree of total length 1200 m

Sakura V1 Serial Pulse Output

The bus is connected to Tankvision or other Endress+Hauser V1- type receiver. The interface or receiver must be configured accordingly.

Termination Resistors

It is not necessary to set any termination resistors.

Bus Address

Each device has an individual bus address and can be set via touch control.

Bus Cabling

The bus cabling is galvanically isolated from the device or interface. Standard communication cable (CPEV or KEPV) can be used.

Bus Topology

The suitable topologies for the serial pulse output are:

Serial max. 6000m (Sakura V1)

Set the V1 so that total extension is within the range of 6000 m per one loop for bus topology.

Enraf Bi Phase Mark Output

The bus is connected to an Enraf I/F CIU or RTU8 to transmit measured value to upper host system as Entis (Enraf TG program) or Fuels Manager. These interface must be configured accordingly.

Termination Resistors

It is not necessary to set any termination resistors for serial pulse output.

Bus Address

Each device has an individual bus address and can be set via touch control.

Bus Cabling

The bus cabling is galvanically isolated from the device or interface adapter. Standard communication cable (CPEV or KEPV) can be used for the data transmission.

Bus Topology

The suitable topologies for Enraf BPM serial pulse output are:

Serial max. resistance: 400 ohm at 3 bus loops or less (10 transmitters per 1bus loop)

Serial max. capacitance: 1 micro F or less

Data Transmission & Operation

NMS5 is capable to transmit following sensory data as well as gauge operation command via Enraf BPM serial pulse output.

- Data: level, temperature, operation status
- Gauge command: STOP, UP, LEVEL, I/F

HART Output

The bus is connected to a HART master. The HART master must be configured accordingly.

Termination Resistors

It is not necessary to set any termination resistors for serial pulse output.

Bus Address

Each device has an individual bus address. This is defined by host system or HART handy terminal.

Bus Cabling

The bus cabling is galvanically isolated from the device and the PC plug-in board or the interface adapter. The screening must be grounded and have electrical continuity throughout. EMC tests indicate the best result when the grounding at both ends and each transmitter is established. If there is a potential difference in between the grounds, measurement must be taken to equalize whilst observing a relevant hazardous area.

Bus Topology

The suitable topologies are:

Serial max. 1000 m

Set HART output so that total extension is within the range of 1000m per one loop for bus topology.

Whessoematic 550 (WM550) Output

The bus is normally connected to Whessoe 1098, RTU 8 or other upper host system via dual channel (can be single) WM550 current loop.

Termination Resistors

It is not necessary to set any termination resistors for serial pulse output.

Bus Address

Each device on a signal loop has an individual bus address. This is defined within the transmitter by mechanical dip switch on communication board.

Bus Cabling

The bus cabling is galvanically isolated from the device and the PC plug-in board or the interface adapter. BS5308 or equivalent 1.5sq.mm screened twisted pairs are recommended for bus cabling.

Bus Topology

The suitable topologies for the WM550 current output are depending on number of transmitter and cable quality on the loop. Recommended number of transmitter on single loop shall be 15 units or less to achieve the maximum performance.

Varec Mark Space (M/S) Output

The bus is normally connected to Interface Unit (IFU), Data acquisition Processor (DAP), RTU 8 or other upper host system via 4 wire M/S serial bus link.

Termination Resistors

It is not necessary to set any termination resistors for serial pulse output.

Bus Address

Each device on a signal loop has an individual bus address. This is defined within the transmitter by mechanical dip switch on com board.

Bus Cabling

The bus cabling is galvanically isolated from the device and the PC plug-in board or the interface adapter. The total length of field wiring shall be determined by calculation of maximum resistance within the system and required operation current. Once the total length is determined, distance has to be reduced by half because of current flow in both B+ & B- leads.

Bus Topology

The suitable topologies for the M/S serial pulse output are depending on number of transmitter & cable quality on the loop.

Operating Conditions: Environment

Ambient Temperature	-20 to +60°C (-4 to 140°F) -40 to +60°C (-40 to 140°F) ATEX approval cold temperature version
Storage Temperature	-40 to +60°C (-40 to 140°F)
Liquid Temperature	-200 to +200°C (-328 to +392°F)
Degree of Protection	IP 67, NEMA4x with closed housing and cable glands
Electromagnetic Compatibility (EMC)	Electromagnetic compatibility meets with EN 61326-1.

Operating Condition: Process

Process Pressure

	Aluminum Drum Housing	Stainless Drum Housing
0 to 19.8kPa (Low Pressure)	NMS5-1	NMS5-2
0 to 588kPa (Medium Pressure)	NMS5-4	NMS5-5
0 to 2.45MPa (High Pressure)		NMS5-6
Maximum process pressure of JIS 10k/ASME Cl. 150/DIN PN10/JPI 150lbs: 0.98MPa		

Measuring Range

Level

28m	Standard Option
36m	Standard Option
47m	Standard Option
Longer ranges available upon request. Contact Endress+Hauser representatives.	

Density

0.430 to 2.000 g/cm³ (g/ml)

Mechanical Construction

Design and Dimensions

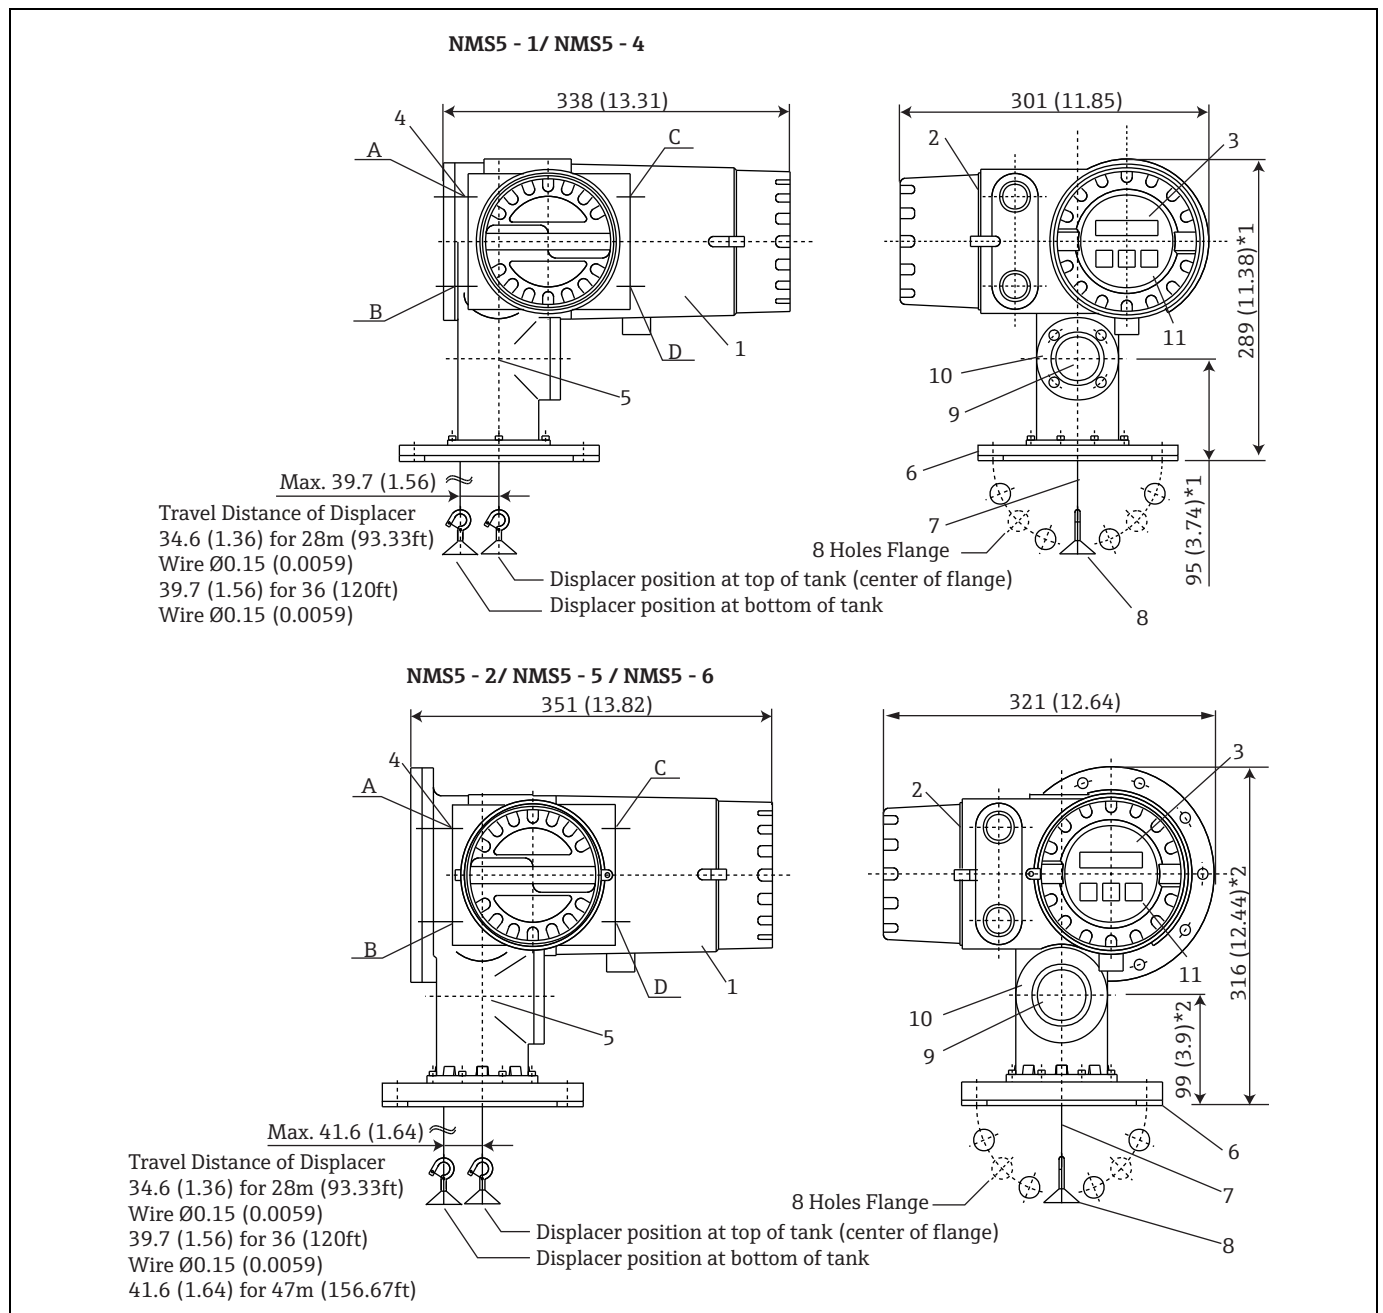


Figure 11: Dimensions of NMS5,
Unit of Measurement: mm (in)

1	Electrical compartment	7	Measuring wire
2	Terminal box	8	Displacer
3	Display (LCD)	9	Calibration window
4	Cable entry (A, B, C, D)	10	Window cover
5	Wire drum housing	11	Touch control
6	Flange		

NOTICE

*1: In case of 18mm (Flange thickness) at JIS10K80ARF

*2: In case of 20mm (Flange thickness) at JIS20K80ARF

Housing Materials of Construction

Electrical compartment: aluminum casting
 Drum chamber for NMS 5-1/5-4: aluminum casting
 Drum chamber for NMS 5-2/5-5/5-6: stainless steel 316 casting

Weight

NMS 5-1/5-4: 12 kg
 NMS 5-2/5-5/5-6: 27 kg

Flange Type

ASME, JIS, DIN 3" and 6" (standard) or equivalent. Refer to order code for full selection.
 Flange for NMS5-1/5-4: aluminum
 Flange for NMS5-2/5-5/5-6: stainless steel 304

Measuring Wire

Material (Standard)

- Stainless steel 316L, 0.15 mm (standard)
- Alloy C. ϕ 0.2 mm (max. 22m range)
- PFA coated SUS316, 0.4 mm (max. 16m range)

⚠ CAUTION

When liquid level in a tank becomes turbulent condition, use a stilling well pipe or a guide wire for installation.

Displacer

- Diameter: 50 mm (Standard), 30 to 110mm (option)
- Material (Standard): Stainless steel 316
- Material (optional): Alloy C, PTFE
- Traveling speed: 0 to 2500 mm /min to maximum

Feature: 070	Measuring Range/Material/ Diameter of Wire	Horizontal Movement Distance (mm/m) on Drum Wire
C	0-28m; SUS316L, 0.15mm	1.24
H	0-16m; PFA>SUS316, 0.4mm	1.34
K	0-16m; Alloy C, 0.2mm	1.57
L	0-36m; SUS316L, 0.15mm	1.10
M	0-22m; Alloy C, 0.2mm	1.57
N	0-47m; SUS316L, 0.15mm	0.88

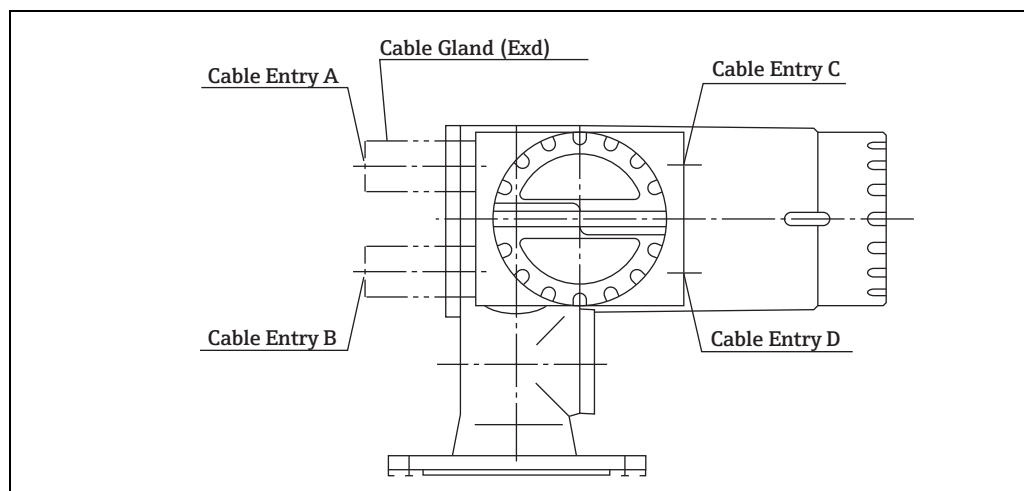
Cable Entry

Figure 12: Cable Entries

⚠ WARNING

When ordering TIIS Ex d specification, cable glands are attached with NMS5. Ensure to use the cable glands.

Human Interface

Operating Concept

NMS5 is furnished with a four line illuminated liquid crystal display. With the E+H matrix driven operation, configuration is simple. Using only three keys, all parameters can be selected and modified. For example:

- Operation - level; interface; spot & profile density, water dip, & tank bottom
- Current output
- Relay output
- Maintenance prediction
- Calibration, etc.

The display can be configured to be displayed in English, Japanese or Chinese. Measurement unit & decimal point can be also configured within NMS matrix.

Operational Security

The programming information can be protected by software access codes that disable all programmable parameters or by a hardware switch to prevent changes from remote transmission or the touch control keypad. A self-diagnosis function checks for any operational failures.

Display (LCD)

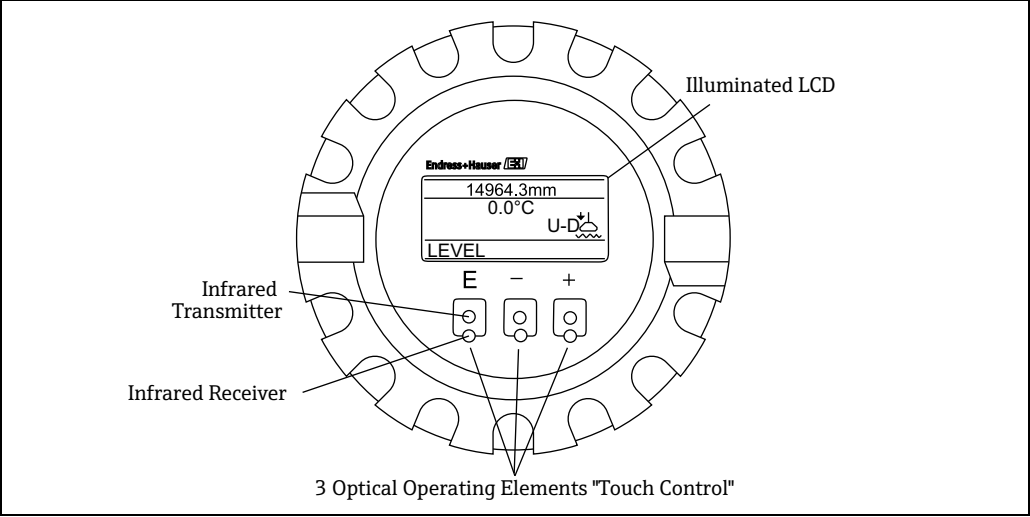


Figure 13: Display (LCD)

Four line 16-digit illuminated display English, Japanese, Chinese selectable

Programming

Three optical keys (touch control) for selection of matrix functions.

Memo Function

Memo of maintenance information.

Advanced Maintenance

Maintenance Prediction	NMS 5 will provide advance warning of required maintenance such as replacement of worn wire etc. The operating life-span of electrical and mechanical parts of the NMS 5 are factory set within the instruments memory. This information is checked involving with the built-in clock and compared and registered in the instrument.
Maintenance	The maintenance record can be accessed via the matrix and will provide information of alarm data (e.g. date, time, alarm type). A memo function allows the user or an E+H Service Engineer to enter maintenance data manually.
Proactive Safety	Proactive safety diagnostic function warns of mechanical failure, and outputs maximum level value, e.g. 99999 to local display and Fieldbus.

Certificates and Approval

CE Mark	By attaching the CE mark, Endress+Hauser confirms that the instruments pass the required tests.
Ex Approvals	TIIS Ex d IIB T4 FM XP Cl. I Div. 1 Gr. C-D FM XP-AIS Cl. I Div.1 Gr. C-D CSA Cl. I Div. 1 Gr. C-D CSA Ex d[ia] Cl. I Div. 1 Gr. C-D ATEX II 1/2G Ex d IIB T6...T3 ATEX II 1/2G Ex d IIC T6...T3 ATEX II 1/2G Ex d IIB T6...T3, -40°C ATEX II 1/2G Ex d (ia) IIB T6...T3 ATEX II 1/2G Ex d (ia) IIB T6...T3, -40°C IEC Ex d ia IIB T6...T3 Ga/Gb IEC Ex d IIB T6...T3 Ga/Gb IEC Ex d IIC T6...T3 Ga/Gb IEC Ex d ia IIB T6...T3 Ga/Gb, -40°C IEC Ex d IIB T6...T3 Ga/Gb, -40°C NEPSI Ex d ia IIB T6...T3 NEPSI Ex d IIB T6...T3 NEPSI Ex d IIC T6...T3 NEPSI Ex d ia IIB T6...T3, -40°C NEPSI Ex d IIB T6...T3, -40°C
Custody Transfer Approvals	PTB: Germany NMI: Netherlands
Overspill Prevention	TÜV: Germany
SIL2	TÜV: Germany
External Standards and Guidelines	EMC-Directive 89/336/EC PE-Directive 97/23/EC EN 10204-3.1B OIML-R85/1998 OIML-R85/2008 SIL IEC61508 ISO 9001:2008

Order Information

NMS5

010	Drum Housing Pressure Rating; Material:		
	1	0... 200mbar/20kPa/2.9psi; Alu	
	2	0... 200mbar/20kPa/2.9psi; stainless ste>	
	4	0... 5.88bar/588kPa/85.28psi; Alu	
	5	0... 5.88bar/588kPa/85.28psi; stainless steel	
	6	0... 24.5bar/2.45MPa/355.34psi; stainless steel	
	9	Special version, TSP-no. to be spec.	
020	Approval:		
	0	Weather proof, IP 67 NEMA 4X	
	1	TIIS Ex d IIB T4	
	5	FM XP Cl. I Div. 1 Gr. C-D	
	N	FM XP-AIS Cl. I Div.1 Gr. C-D	
	6	CSA Cl. I Div. 1 Gr. C-D	
	O	CSA Ex d ia Cl. I Div. 1 Gr. C-D	
	G	ATEX II 1/2G Ex d IIB T6...T3	
	Q	ATEX II 1/2G Ex d IIC T6...T3	
	S	ATEX II 1/2G Ex d IIB T6...T3, -40°C	
	J	ATEX II 1/2G Ex d (ia) IIB T6...T3	
	U	ATEX II 1/2G Ex d (ia) IIB T6...T3, -40°C	
	A	IEC Ex d ia IIB T6...T3 Ga/Gb	
	B	IEC Ex d IIB T6...T3 Ga/Gb	
	C	IEC Ex d IIC T6...T3 Ga/Gb	
	D	IEC Ex d ia IIB T6...T3 Ga/Gb, -40°C	
	E	IEC Ex d IIB T6...T3 Ga/Gb, -40°C	
	T	NEPSI Ex d ia IIB T6...T3	
	V	NEPSI Ex d IIB T6...T3	
	W	NEPSI Ex d IIC T6...T3	
	X	NEPSI Ex d ia IIB T6...T3, -40°C	
	4	NEPSI Ex d IIB T6...T3, -40°C	
	9	Special version, TSP-no. to be spec.	
030	Application:		
	A	Liquid Level	
	B	PTB (<1mm) type approval, liquid level	
	C	NMi (<1mm) type approval, liquid level	
	D	Multi measurement, liquid level, I/F level, bottom, density	
	E	PTB (<1mm) type approval, liquid level, I/F level, bottom, density	
	F	NMi (<1mm) type approval, liquid level, I/F level, bottom, density	
	G	Density profile multi measurement, liquid level, I/F level, bottom, density	
	H	PTB (<1mm)type approval, density profile, liquid level, I/F level, bottom, density	
	J	NMi (<1mm) type approval, density profile, liquid level, I/F level, bottom, density	
	Y	Special version, TSP-no. to be spec.	
040	Output 1:		
	F	Not selected	
	A	2-way 2-wire (V1 protocol)	
	J	2-way 2-wire (MDP protocol)	
	B	2-way 2-wire (BBB protocol)	
	C	2-way 2-wire (MIC, RS232C protocol)	
	D	2-way 2-wire (MIC protocol)	
	G	HART active	
	H	HART passive	
	L	Whessmatic 550, overvoltage protection	
	M	Mark Space	
	N	Enraf BPM	
	P	Modbus RS 485	
	Y	Special version, TSP-no. to be spec.	
NMS5-			Product designation (Continued on next page)

31

Accessories

Calibration Chamber

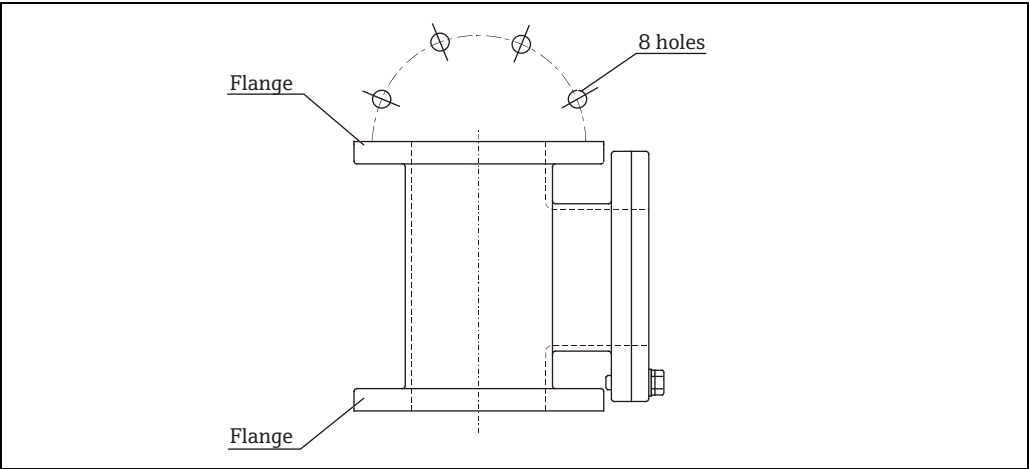


Figure 14: Calibration Chamber, Unit of Measurement: mm (in)

Calibration chamber is recommended for use with tank level gauges in order to allow maintenance (removing displacers), while tank is in service.
Standard chamber is 6" flange, with bolts and packing for NMS connection.

NOTICE

The dimensions differ depending on material, flange size. Contact Endress+Hauaser for details.

NHC4HP (High Pressure Version)

010	Process Connection:		
	A	10K 150A RF, flange JIS B2220	
	C	10K 150A FF, flange JIS B2220	
	E	20K 150A RF, flange JIS B2220	
	G	NPS 6" Cl.150 RF, flange ASME B16.5	
	J	NPS 6" Cl.300 RF, flange ASME B16.5	
	L	DIN 150 PN10 B1, flange EN1092-1(DIN2527 B)	
	N	DIN 150 PN25 B1, flange EN1092-1(DIN2527 B)	
	Q	150A 150lbs RF, flange JPI 7S-15	
	S	150A 300lbs RF, flange JPI 7S-15	
	Y	Special version, TSP-no. to be spec.	
020	Pipe Material; Flange Material:		
	2	STPG370; SS400	
	3	SUS304TP; SUS304	
	9	Special version, TSP-no. to be spec.	
030	Bolts, Packing:		
	0	not used	
	1	SUS304, Valke #6502	
	9	Special version, TSP-no. to be spec.	
040	Pressure Gauge, Relief Valve:		
	1	Selected	
	9	Special version, TSP-no. to be spec.	
NHC4HP-			Complete product designation

NHC4LP (Low Pressure Version)

010	Process Connection:		
	A	10K 150A RF, flange JIS B2220	
	C	10K 150A FF, flange JIS B2220	
	G	NPS 6" Cl.150 RF, flange ASME B16.5	
	L	DN150 PN10 B1, flange EN1092-1(DIN2527 B)	
	Q	150A 150lbs RF, flange JPI 7S-15	
	Y	Special version, TSP-no. to be spec.	
020	Pipe Material; Flange Material:		
	1	AC4A ; AC4A	
	3	SUS304TP ; SUS304	
	9	Special version, TSP-no. to be spec.	
030	Bolts, Packing:		
	0	not used	
	1	SUS304, Walker #6502	
	9	Special version, TSP-no. to be spec.	
NHC4LP-			Complete product designation

Power + Control Switch

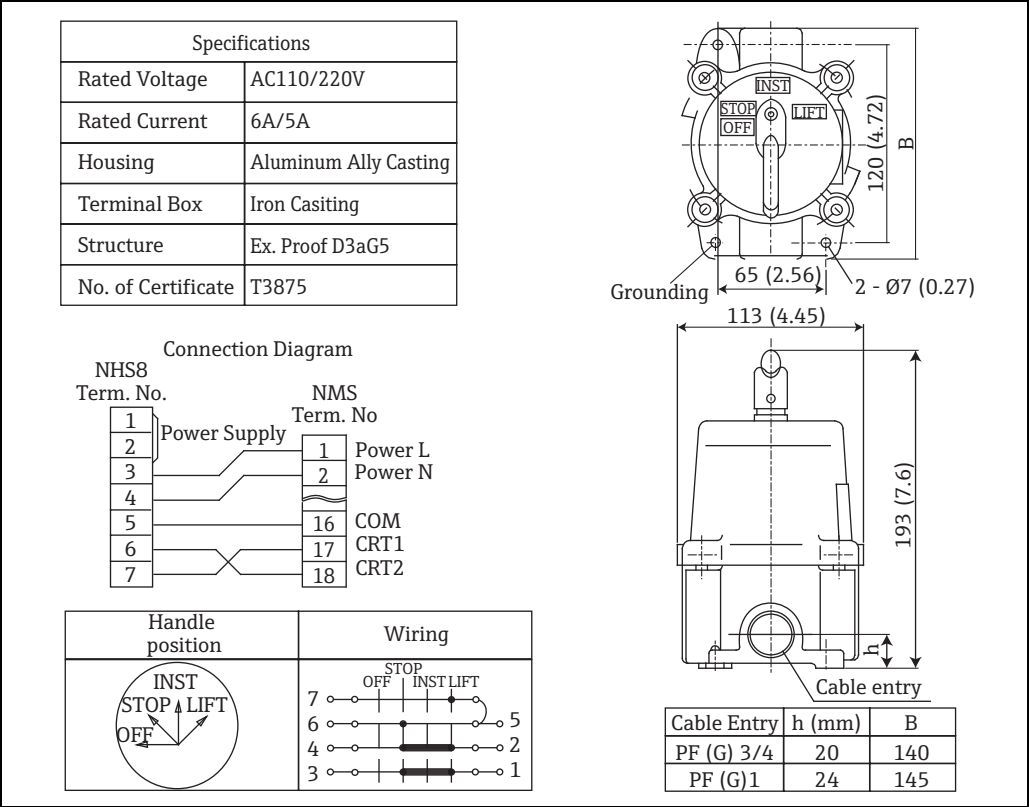


Figure 15: Power and Control Switch, Unit of Measurement: mm (in)

Power & Control Switches are used for field mounted tank gauges. This provides additional gauge operation contact switching in order to control gauge’s operation, such as hoisting up displacer.

NHS8

010	Approval:	
	1	Weather proof IP67
	2	Flame proof (TIIS d3aG5)
020	Cable entry:	
	0	2 x thread G3/4
	1	2 x thread G1
	2	2 x thread NPT3/4
	3	2 x thread NPT1
	9	Special version, TSP-no. to be spec.
NHS8-		Complete product designation

Ball Valve

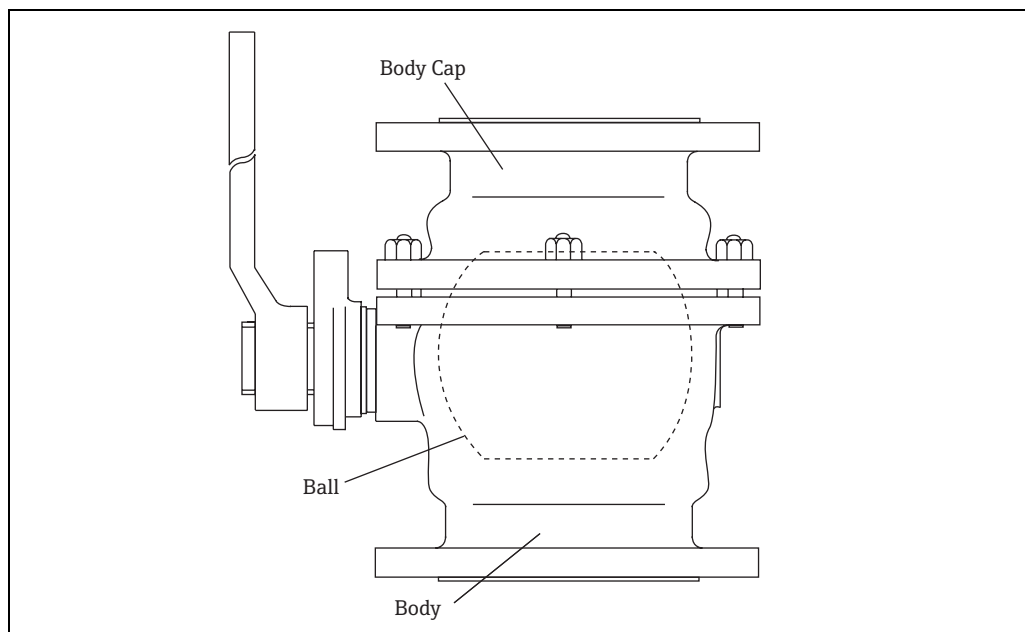


Figure 16: Parts Name of Ball Valve

Ball valves are recommended for use with tank level gauges in order to allow such maintenance as removing displacers, while tank is in service.

Standard ball valve with ASME flanges. Ball material is SS304, seat material is PTFE.

NOTICE

The dimensions vary depending on material, flange size. Contact Endress+Hauser for details.

NHV4A (ASME flanges)

Standard ball valve with ASME flanges. Ball material is SS304, seat material is PTFE.

010	Process Connection; Body:	
C31	NPS 3" Cl.150 RF; steel casting flange ASME B16.5	
C33	NPS 3" Cl.300 RF; steel casting flange ASME B16.5	
C61	NPS 6" Cl.150 RF; steel casting flange ASME B16.5	
C63	NPS 6" Cl.300 RF; steel casting flange ASME B16.5	
S31	NPS 3" Cl.150 RF; SUS304 flange ASME B16.5	
S33	NPS 3" Cl.300 RF; SUS304 flange ASME B16.5	
S61	NPS 6" Cl.150 RF; SUS304 flange ASME B16.5	
S63	NPS 6" Cl.300 RF; SUS304 flange ASME B16.5	
Y99	Special version, TSP-no. to be spec.	
020	Ball Type:	
A	Full bore	
B	Reduced bore	
Y	Special version, TSP-no. to be spec.	
NHV4A-	Complete product designation	

NHV4J (JIS flanges)

For body in mild steel and in SS304, ball material is SS304, ball material is SS304. For body in SS316, ball material is SS316. Seal material is PTFE.

10	Process Connection; Body:	
	C11	10K 80A RF; Steel flange JIS B2220
	C12	10K 150A RF; Steel flange JIS B2220
	C21	20K 80A RF; Steel flange JIS B2220
	C22	20K 150A RF; Steel flange JIS B2220
	S11	10K 80A RF; SUS316 flange JIS B2220
	S12	10K 150A RF; SUS316 flange JIS B2220
	S21	20K 80A RF; SUS316 flange JIS B2220
	S22	20K 150A RF; SUS316 flange JIS B2220
	H11	10K 80A RF; SUS304 flange JIS B2220
	H12	10K 150A RF; SUS304 flange JIS B2220
	H21	20K 80A RF; SUS304 flange JIS B2220
	H22	20K 150A RF; SUS304 flange JIS B2220
	Y99	Special version, TSP-no. to be spec.
20	Ball Type:	
	A	Full bore
	B	Reduced bore
	Y	special version, TSP-no. to be spec.
NHV4J-		Complete product designation

Reducing Flange

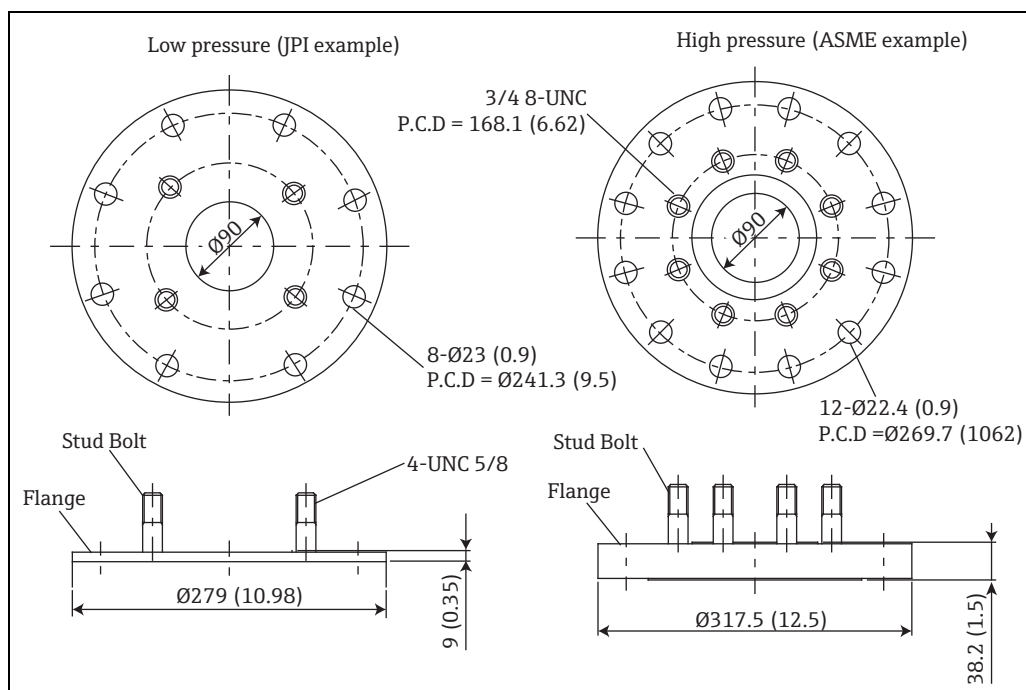


Figure 17: Reducing Flange, Unit of Measurement: mm (in)
 Use reducing flange when NMS5 connection 80A(30") and mounting nozzle is 150A(6").

NHF4

10	Process Connection; Body:	
	A	10K 150A RF, flange JIS B2220
	C	10K 150A FF, flange JIS B2220
	E	20K 150A RF, flange JIS B2220
	G	NPS 6" Cl.150 RF, flange ASME B16.5
	J	NPS 6" Cl.300 RF, flange ASME B16.5
	L	DIN 150 PN10 B1, flange EN1092 (DIN2527 B)
	N	DIN 150 PN25 B1, flange EN1092 (DIN2527 B)
	Q	150A 150lbs RF, flange JPI 7S-15
	S	150A 300lbs RF, flange JPI 7S-15F
	Y	Special version, TSP-no. to be spec.
20	Flange Material:	
	0	SS400
	1	SUS304
	9	Special version, TSP-no. to be spec.
NHF4-		Complete product designation

NOTICE

NHF4 is not required if NMS5 is ordered with "Order Information; Guide Wire Installation (130-E)". When NHF4 is ordered as NMS5-xxxxxxxxxxxE with Guide Wire Installation, all the required mounting equipment is included.

Supplementary Documentation

Technical Information	TI00042G Prothermo NMT 539
	TI00462G Promonitor NRF 560
Operating Manual	BA00401G Proservo NMS5
Compact Instructions	KA001N Whessoemtric 550
	KA002N RS485 Modbus
Safety Instructions	XA00578G Proservo NMS5 - ATEX
	XA00582G Proservo NMS5 - IECEx
	XA10257G Proservo NMS5 - NEPSI
	EX421-439 Proservo NMS5 - FM
	EX540-742 Proservo NMS5 - CSA
Functional Safety Manual	SD00337G Proservo NMS5 - (4-20mA Output, Overspill prevention relay)

Appendix

Stainless Steel Conversion Table

The stainless steel material used in products of Endress + Hauser Yamanashi normally have expressions according to Japanese industrial standards, such as JIS. Each country or region may have different expressions place to place.

The following conversion table contains the expression of equivalent stainless steel material based on the chemical composition and mechanical properties.

County	Standard	Expressions			
Japan	JIS	SUS304	SUS304L	SUS316	SUS316L
Germany	DIN 17006	X5 CrNi 18 10 X5 CrNi 18 12	X2 CrNi 18 11	X5 CrNiMo 17 12 2 / 17 13 3	X2 CrNiMo 17 13 2
	W.N. 17007	1.4301 1.4303	1.4306	1.4401 / 1.4436	1.4404
France	AFNOR	Z 6 CN 18-09	Z 2CN 18-10	Z 6 CND 17-11 / 17 12	Z2 CND 17-12
Italy	UNI	X5 CrNi 1810	X2 CrNi 1911	X5 CrNiMo 1712 / 1713	X2 CrNiMo 1712
U.K.	BSI	304S15 / 304S16	304S11	316S31 / 316S33	316S11
U.S.A.	AISI	304	304 L	316	316L
U.E.	EURONORM	X6 CrNi 1810	X3 CrNi 1810	X6 CrNiMo 17 12 2 / 17 13 3	X3 CrNiMo 17 12 2
Spain	UNE	X6 CrNi 19-10	X2 CrNi 19-10	X6 CrNiMo 17-12-03	X2 CrNiMo 17-12-03
Russia	GOST	08KH18N10 06KH18N11	03KH18N11	—	03KH17N14M2
-	ISO	11	10	20	19
-	ASME	S30400	S30403	S31600	S31603

NOTICE

Since each standard carries its own mechanical and scientific definition, some expressions on the list above may not have a straight conversion from the Japanese standard. Consult a local authority or legislature to ensure proper comparison of the applied standard prior to determining specifications.

www.addresses.endress.com

For more Endress+Hauser product please visit: www.ainstru.com
Mail: Sales@ainstru.com